

**NASA CONTRACTOR
REPORT**



NASA CR - 54085

NASA CR - 54085

FACILITY FORM 608	N65-11004	
	(ACCESSION NUMBER)	(THRU)
	43	7
	(PAGES)	(CODE)
	CR 54085	02-14
	(NASA CR OR TMX OR AD NUMBER)	(CATEGORY)

**LIQUID HYDROGEN
FILM COOLED PRESSURE TRANSDUCERS**

By J. Delmonte

*Prepared under Contract No. NAS3-2754 by
ELECTRO-OPTICAL SYSTEMS, INC.
Pasadena, California*

0

NOTICE

This report was prepared as an account of Government sponsored work. Neither the United States, nor the National Aeronautics and Space Administration (NASA), nor any person acting on behalf of NASA:

- A.) Makes any warranty or representation, expressed or implied, with respect to the accuracy, completeness, or usefulness of the information contained in this report, or that the use of any information, apparatus, method, or process disclosed in this report may not infringe privately owned rights; or
- B.) Assumes any liabilities with respect to the use of, or for damages resulting from the use of any information, apparatus, method or process disclosed in this report.

As used above, "person acting on behalf of NASA" includes any employee or contractor of NASA, or employee of such contractor, to the extent that such employee or contractor of NASA, or employee of such contractor prepares, disseminates, or provides access to, any information pursuant to his employment or contract with NASA, or his employment with such contractor.

Requests for copies of this report should be referred to

National Aeronautics and Space Administration
Office of Scientific and Technical Information
Attention: AFSS-A
Washington, D.C. 20546

CASE FILE COPY

9

CONTRACTOR REPORT

LIQUID HYDROGEN FILM COOLED PRESSURE TRANSDUCERS

By J. Delmonte

Prepared under Contract NAS3-2754
Electro-Optical Systems, Inc.
300 North Halstead Street
Pasadena, California

December 1964

Technical Management
Mr. James W. Norris

Lewis Research Center

Cleveland, Ohio

NATIONAL AERONAUTICS AND SPACE ADMINISTRATION

CONTENTS

	<u>Page</u>
SUMMARY	
1. INTRODUCTION	1
2. TECHNICAL DISCUSSION	3
2.1 Prototype program for 300°K to 20°K operational pressure transducer capable of being cooled by liquid hydrogen	3
2.2 Work accomplished between March 15 and April 25	8
2.3 Review of Statement of Work	13
3. RECOMMENDATIONS	16
3.1 Mechanical features of EOS PT15C-2 design	16
3.2 Four-active-element silicon chip beam	17
3.3 Thermal Environment: Transient and Steady State	17
4. CONCLUSION	18
APPENDIX I -LIST OF ABBREVIATIONS	
APPENDIX II -FABRICATION OF SINGLE CHIP BEAMS IN SILICON	
APPENDIX III -TABLES 1, 2, 3 and 4	
APPENDIX IV -PT15C-2 PARTS LIST	

ILLUSTRATIONS

<u>Figure</u>		<u>Page</u>
1	PT15C-2 pressure transducer	2
2	Layout of diffused four-active arm silicon strain gage beam chip	4
3	Silicon chip with full bridge diffused into surface. Size 0.040 in. x 0.060 in.	5
4	Four-active arm silicon chips on 304 SS, some silicon chips bonded, some suspended off the metal bar	7
5	Multiple element silicon chip mounted on Invar constant stress beam	7
6	Top assembly - Pressure Transducer model PT15C-2	9
7	Installation and calibration - Ser. No. 2, PT15C-2	10
8	Installation and calibration - Ser. No. 3, PT15C-2	11
9	Installation and calibration - Ser. No. 4, PT15C-2	12
10	Laboratory and field test apparatus and pressure system	14
11	EOS developed PT15B combustion pressure transducer with coolant flow in operation just prior to flame impingement	19
12	Oxy-hydrogen flame impingement directly on diaphragm of PT15B combustion pressure transducer	20
13	Preliminary information on installation of film cooled (H ₂ O) combustion pressure transducer PT15B-2	21

11004

SUMMARY

Abet

The first generation construction and test of three cryogenic-cooled combustion pressure transducers capable of transducing steady state as well as high frequency pressure pulses have been successfully accomplished. These are embodied in Electro-Optical Systems pressure transducers PT15C-2, Serial Nos. 2, 3, and 4, as outlined in Print B 500160-2 Revision 3 of subject contract. Figure 1 is a photograph of the finished transducer.

Optimization of electrical output, leading to improved performance specifications, and reassessment of installation details, reflecting in increased handling strength and field reliability, will result in accurate, rugged, and reliable instrumentation capable of surviving combined environment extremes, with increased output.

The efficiency of film cooling the PT15C-2 transducer with liquid hydrogen is yet to be proven under combustion pressure and temperature conditions. Static tests performed to date indicate that bridge-type solid state pressure transducers are capable of creditable performance to at least LH_2 temperatures with controllable output (sensitivity) and zero shift. Size adaptability, low weight, good output strength, and electrical simplicity are salient features of this type of pressure instrumentation.

Author

1. INTRODUCTION

This document constitutes the final report on NAS3-2754 contract. It covers the specific span of time from March 15, 1964 through the week ending April 25, 1964, as well as documents and summarizes the results of the entire contract work. It includes recommendations and conclusions based upon the experience and results obtained.

To Messrs. S. Kaye of the Semiconductor Department and Wm. McLellan of the Mechanical Engineering Department is due much appreciation for the expediency in developing the highly-doped four-active arm silicon strain gage configuration and tests thereon, within their respective laboratories at Electro-Optical Systems, Inc. Mr. J. Frassrand of the Electro-Optical Systems, Inc. transducer laboratory exhibited unusual skill in fabrication and assembly techniques.

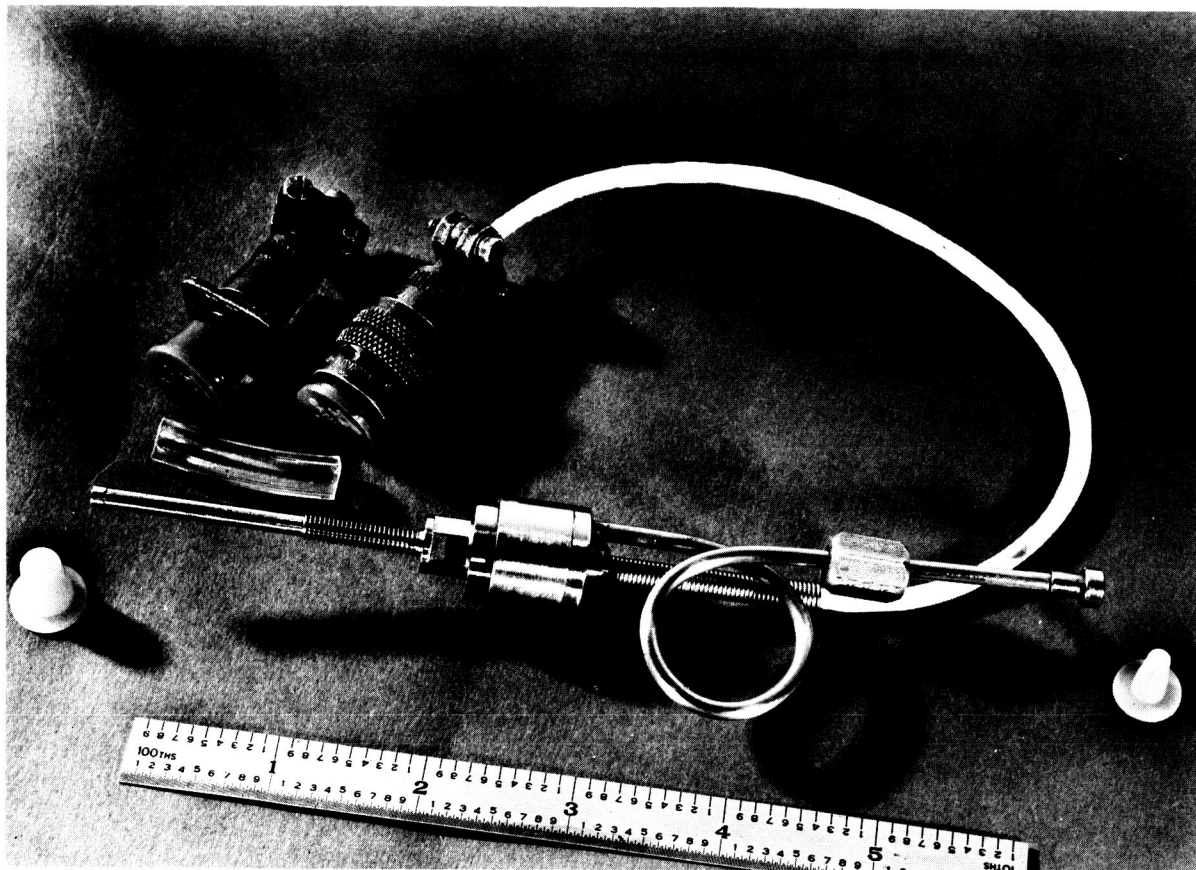


FIG. 1 PT15C-2 PRESSURE TRANSDUCER

2. TECHNICAL DISCUSSION

2.1 Prototype program for 300°K to 20°K operational pressure transducer capable of being cooled by liquid hydrogen.

Phase I: From basic technologies previously pursued at Electro-Optical Systems and its subsidiary, Micro Systems, Inc., the diffused four-active element solid state piezoresistive gage beam had been successfully proven and transducer* tested.

However, to span the temperatures required of this project an exhaustive literature search had to be instituted by the Semiconductor Department under Mr. S. Kaye, and many intensive trail and error tests accomplished within a relatively short time to produce acceptable silicon strain gage elements with the proper mechanical configuration, electrical resistance, temperature coefficient of resistance, and gage factor. Handling characteristics for contacting an ultimate bonding had to be reduced to the level of the skill of average assembly technicians.

A best compromise condition, resulted in relatively high P dopant level diffusion into the bulk silicon, a lowered gage factor of about 50, at room temperature, and a relatively low temperature coefficient of resistance for the four individual resistances. Mr. Kaye has prepared a section on fabrication of single chip beams in silicon, having four active strain gage arms. See Appendix II in which four significant references are cited.

Final chip configuration is illustrated in Fig. 2; an actual photograph of the four-active element gage is to be seen in Fig. 3.

Phase II: Testing the silicon element from the transducer viewpoint of end use:

This involved the mechanical, thermal, and electrical integration of the silicon chip with a suitable pressure summing device. The latter, an integrally machined clamped diaphragm, was already defined, size-wise, not to exceed 0.115 inch diameter, because of previous constraints imposed by the available entry geometry to the rocket combustion chamber.

*Electro-Optical Systems Patent application pending.

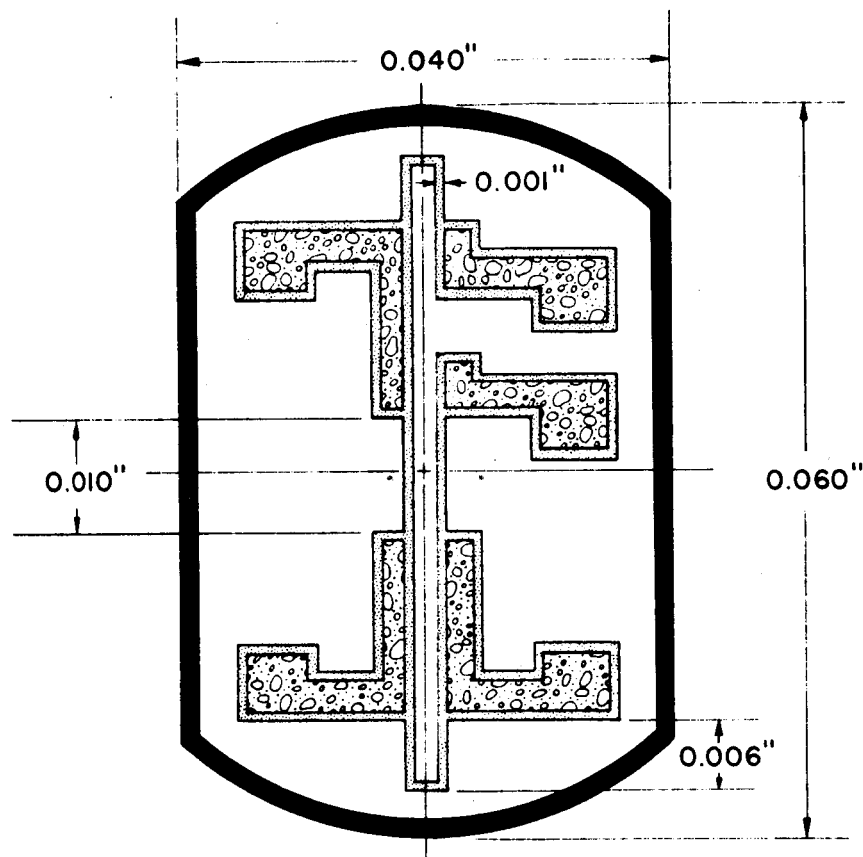


FIG. 2 LAYOUT OF DIFFUSED FOUR-ACTIVE ARM SILICON STRAIN GAGE BEAM CHIP

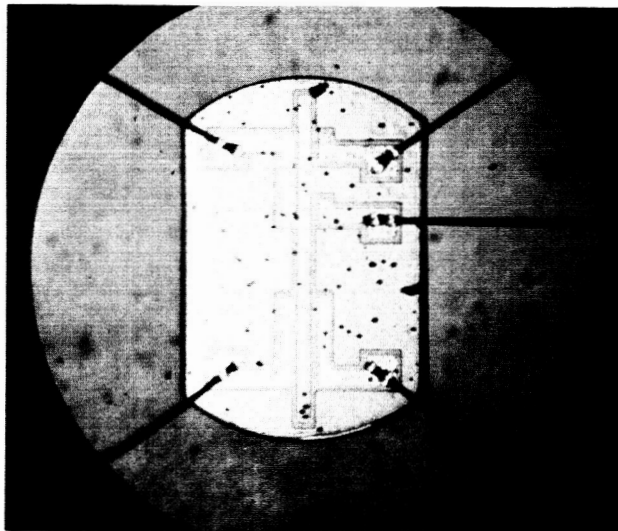


FIG. 3 SILICON CHIP WITH FULL BRIDGE
DIFFUSED INTO SURFACE.
SIZE 0.040 IN. X 0.060 IN.

Integrity of the silicon chip was assured by shock testing to LH_2 and intermediate temperatures, repeatedly, and recording the changes in its four resistances, in the unbonded and bonded condition. This was accomplished both at EOS's transducer laboratory and at the Norco facility of Wyle Laboratories. Typical data accumulated from these tests is shown in Table 1 of Appendix III.

Figure 4 shows the 304 SS test setup.

Figure 5 depicts the chip mounted on Invar constant stress beam.

Knowing that the silicon element responds either more or less linearly with its original "clamping" stress (a function of the adhesive used, the cure temperature, and the difference in thermal contraction between silicon and the diaphragm metal), we decided to bracket thermal expansion coefficient of the silicon chip by mounting it on a 300 series stainless steel diaphragm and comparing the results with that of an Invar steel diaphragm.

The following set of conditions was investigated:

Silicon chip bonded to 304 SS: flat bar; diaphragm

Silicon chip bonded to Invar: constant stress beam; diaphragm

Silicon chip bonded to NiSpan C: diaphragm

Tests were conducted at LO_2 - LN_2 , CO_2 and LH_2 temperatures, repeatedly. Typical data is tabulated in Tables 2 and 3, Appendix III.

That the silicon chip geometry did not require altering and its electrical characteristics and performance with a variety of metals behaved according to prediction attests to the fundamental integrity of the semiconductor element, the contacting and bonding methods employed. (TCB-aluminum contacting leads were used to join to the silicon element in all the above tests.)

Phase III was the actual buildup of a small group of complete pressure transducers, testing and electrically compensating for operation between LH_2 and room temperature.

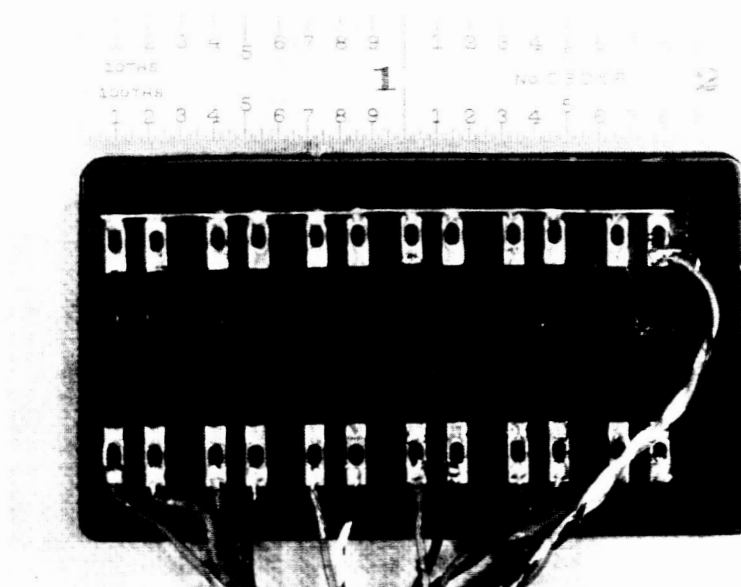


FIG. 4 FOUR-ACTIVE ARM SILICON CHIPS ON 304 SS,
SOME SILICON CHIPS BONDED, SOME SUSPENDED
OFF THE METAL BAR

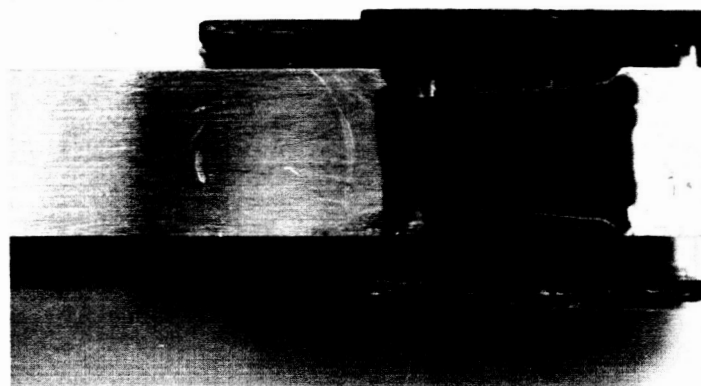


FIG. 5 MULTIPLE ELEMENT SILICON CHIP MOUNTED ON
INVAR CONSTANT STRESS BEAM

Figure 6, Drawing D-427021, shows the top assembly construction of the EOS PT15C-2 combustion pressure transducer.* Installation and calibration information is included in Figs. 7, 8, and 9. Actual calibration test details for Serial Nos. 2, 3, and 4 are included in Appendix III, Table 4. Appendix IV tabulates a complete parts list.

2.2 Work accomplished between March 15 and April 25:

The buildup and final calibration runs of four transducers were partially accomplished during this period. Three of the four survived intact calibration through liquid nitrogen temperatures at EOS. They were PT15C-2 Serial Nos. 2, 3, and 4.

For field calibration runs to LH_2 , we elected to partially pot the compensation network with a coating of RTV silastic resin to protect the final cable interconnect wires, balance, zero shift, and sensitivity compensating resistors, from humidity changes and vibration fatigue effects. However, upon testing the units at LH_2 for the first time at the Norco facility of Wyle Laboratory, all these units developed minor difficulties which were not correctable in the field.

Unit No. 2: bridge intact; compensation network open

Unit No. 3: bridge intact; compensation network intact;
gold seal leak

Unit No. 4: bridge intact; compensation network open

Upon returning to EOS, all three were made operational and checked again at LN_2 . All closely repeated their original drift, sensitivity, and linearity characteristics from RT to LN_2 , and return to room temperature. This time no potting was used to protect the compensation network other than brush coating with a heat-cured furane thermoset adhesive. Placement of the fixed bridge compensation resistors so that they would be protected against gross shock mishandling was emphasized.

* Note that the original 0.170-inch front diameter was further reduced to 0.150 inch. This change would aid in the installation entry machining problems by presenting a transducer dimension less than the minor diameter of the threaded 10-32 boss (0.156 inch) and still reduce the area of direct heat impingement in the combustion zone.

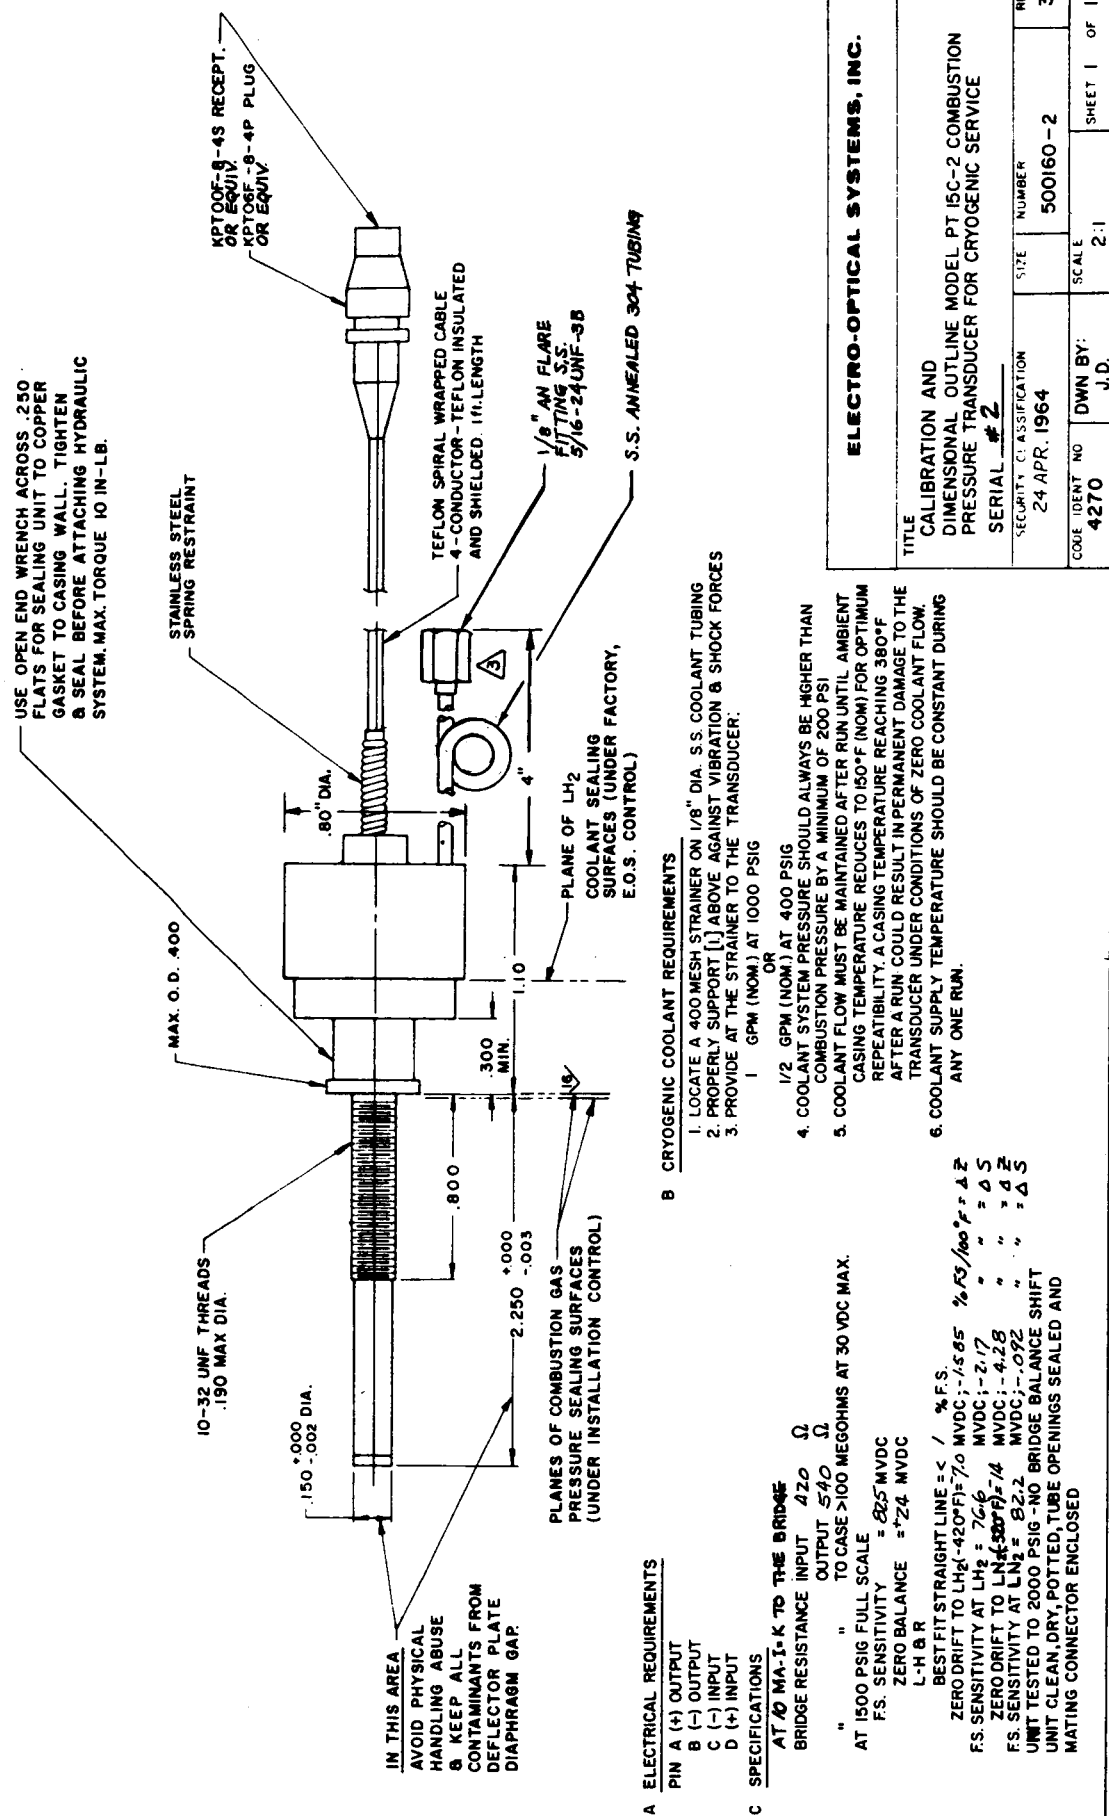


FIG. 7 INSTALLATION AND CALIBRATION - SER. NO. 2, PT15C-2

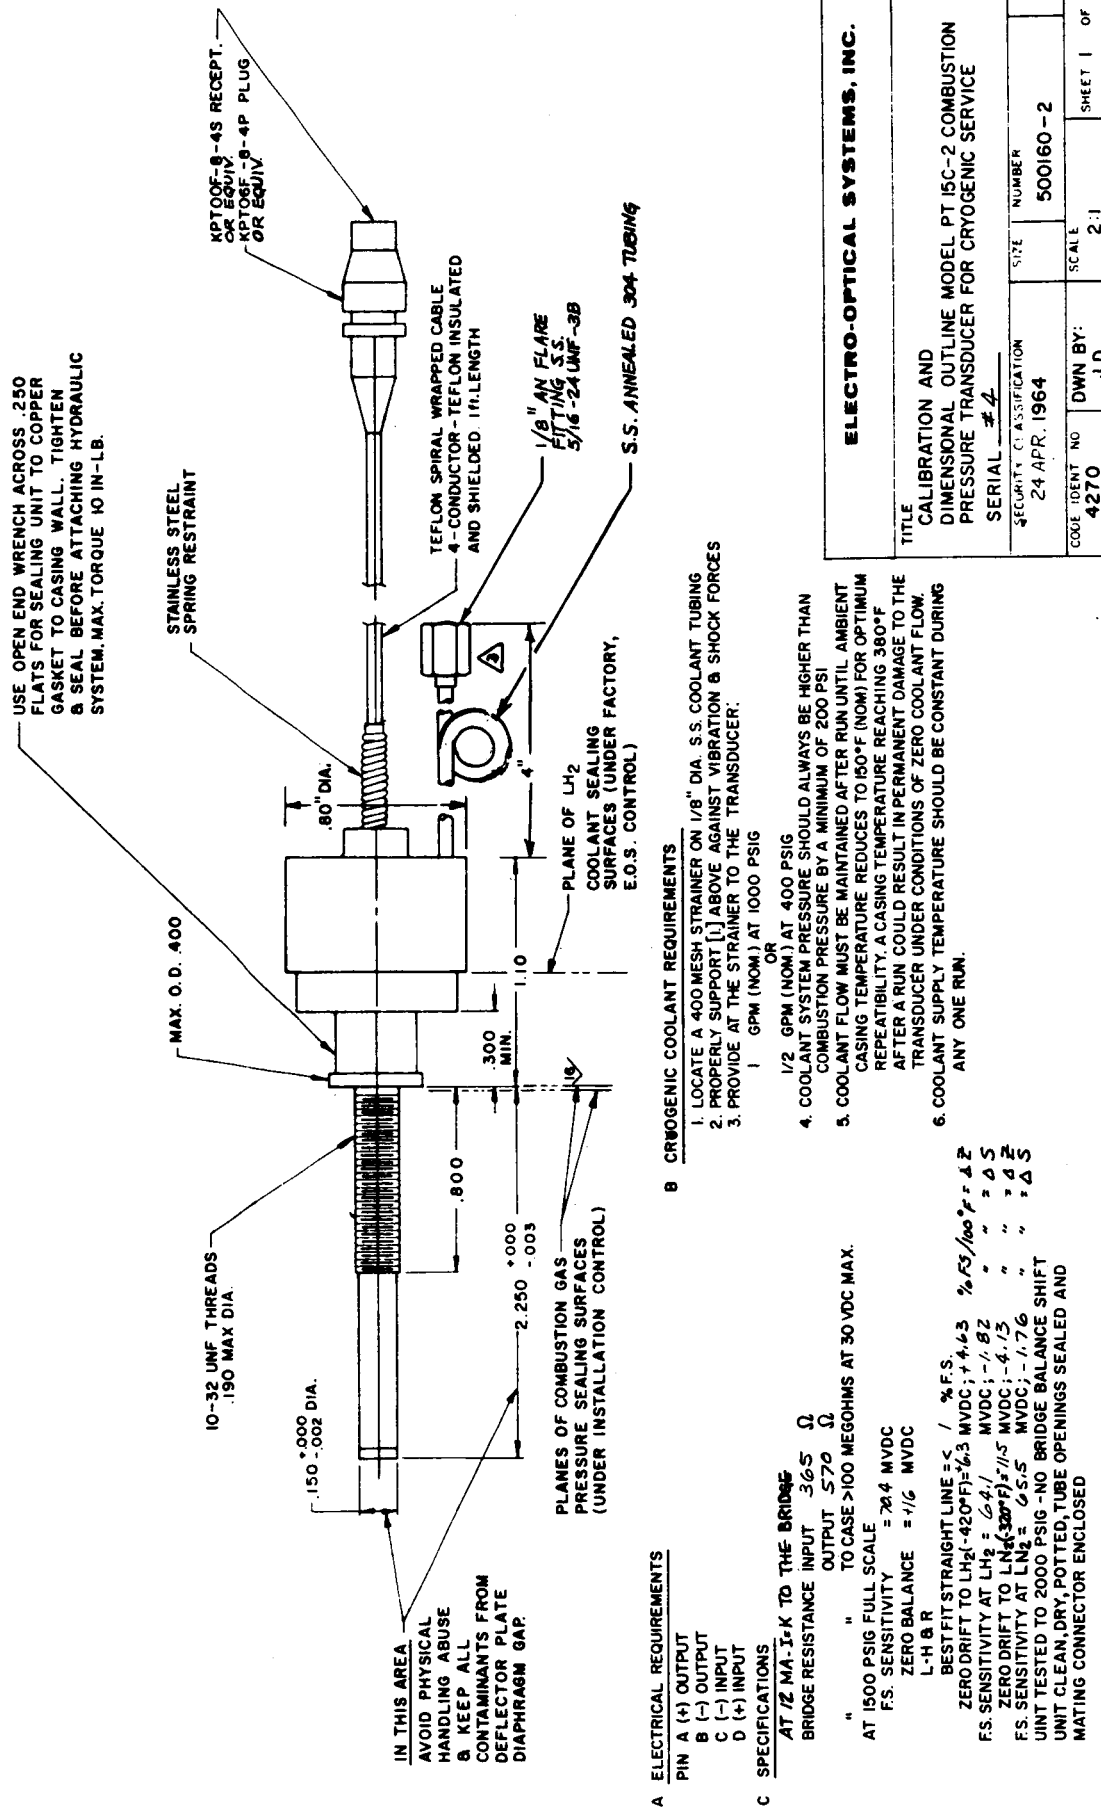


FIG. 9 INSTALLATION AND CALIBRATION - SER. NO. 4, PT15C-2

On the second series of tests at Norco on April 22, all three units were successfully calibrated at LH_2 temperatures without mishap. High pressure helium gas was the pressurizing medium and was simultaneously introduced into the dead weight testing lines and into the LH_2 submerged transducer coolant tube, then through the transducer into a fixed stainless steel trapped volume which was threaded on the 10-32 threads, and pressure sealed against the 0.400-inch diameter flange area (see Fig. 10).

Final checkout at EOS disclosed no internal moisture condensation problem and complete return to normal room temperature calibration condition. All three transducers were thoroughly cleaned, vacuum dried, open tube endings capped and made ready for shipment to the contractor.

2.3 Review of Statement of Work:

In the design, fabrication and test of three cryogenic film cooled pressure transducers, the following statements are made in a numerical sequence to coincide with the specific Work Statement, item for item:

1. The only construction materials in contact with liquid hydrogen are stainless steels (300 series), nickel steel (NiSpanC), copper, and copper brazing alloys.
2. Sensing element is the piezoresistive type strain gage constructed upon high purity elemental silicon.
3. All the transducers will withstand pressure to 2,000 psig without recalibration and without causing permanent change in transducer characteristics.
4. Active working diameter of the flush-mounted transducers is 65 mils exposed to the rocket chamber environment.
5. Mounting: as described in B-500160 drawing (Fig. 6)
6. Pressure range: 0 to 1500 psig.
7. Frequency response: flat from dc to 10 kc; undamped natural frequency by calculation is > 100 kc.

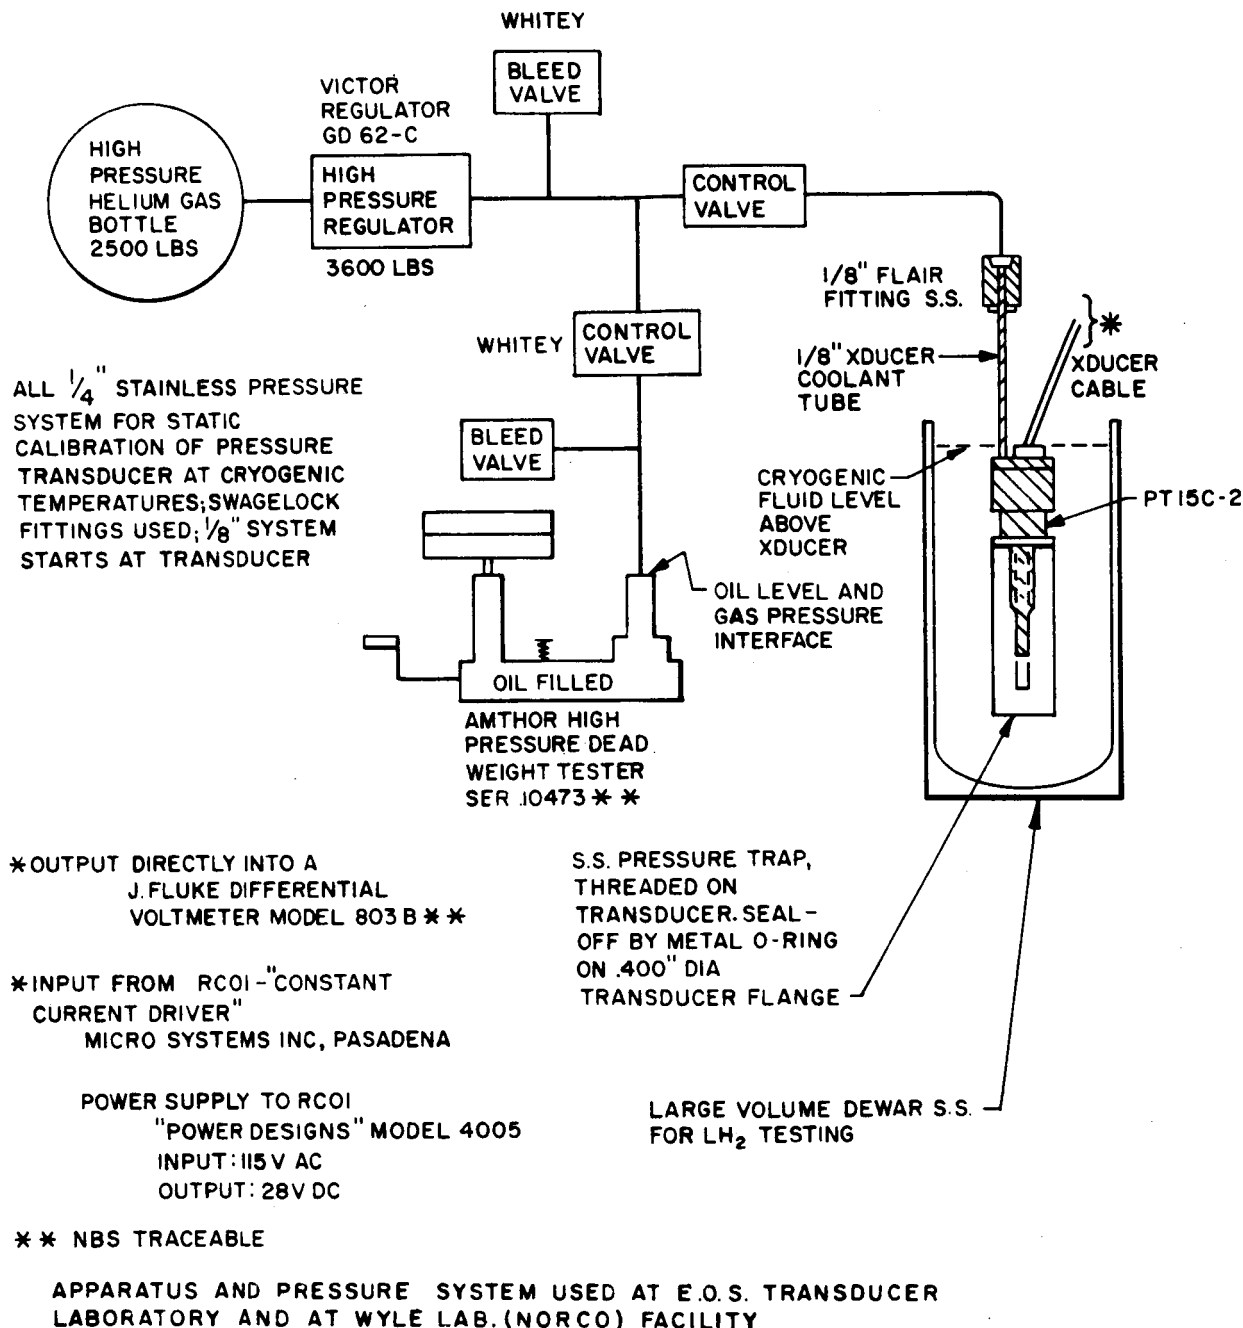


FIG. 10 LABORATORY AND FIELD TEST APPARATUS AND PRESSURE SYSTEM

8. Combined accuracy: L-H and R = < 1 percent F.S. (at steady state temperature condition).
9. Full scale output: > 60 mvdc, unamplified.
10. Excitation voltage: < 10 vdc
Constant current: < 15 Ma
Bridge impedance: < 1000 ohms
See individual calibration sheet, Figs. 7, 8, and 9 and Table 4, Appendix III.
11. Liquid H_2 has heat of vaporization = 194.22 Btu/lb, at one atmosphere pressure; and
12. By forcing liquid H_2 through the unit at greater than combustion pressures and at a rate of 1 to 2 gallons a minute, the four-active arm silicon sensor should survive and not heat up under large heat fluxes. Liquid coolant must be passed through the transducer at least 30 to 60 seconds before combustion is initiated to stabilize the active bridge and fixed compensating network. Coolant must continue to flow after combustion cutoff until motor casing cools below 300°F.
13. Bridge zero-drift and bridge sensitivity drift have been examined at LN_2 and LH_2 . Whereas it is possible to achieve ± 1 percent full scale per 100°F at one cryogenic temperature (LH_2); it seems more practical to open this specification slightly until testing at LH_2 becomes more commonplace. See individual calibration sheets, Figs. 7, 8, and 9, and further remarks under Section D, Recommendations.

In summation, three pressure transducers have been designed, built, and tested for operation at LH_2 conditions to a specific entry-mounting geometry and have successfully fulfilled all the basic requirements of the contract Work Statement.

3. RECOMMENDATIONS

3.1 Mechanical Features of EOS' PT15C-2 Design

3.1.1 Although it can be demonstrated that a geometry employing 10-32 threads in the mounting area is not unreasonable to achieve, it is more realistic to admit that it is also too easy to damage these threads by inadvertent overtightening. The LH_2 cooled combustion pressure seal must be metal, and the natural tendency is to overtighten. We recommend that where possible a motor chamber internal threaded boss of 7/16-20 size be used and threaded to a controlled depth, thence to a small through bore into the combustion chamber. This would have the result of distinct improvement in field handling and reliability of the transducer installation.

3.1.2 The internal cryogenic coolant seal and the external combustion gas seal areas should be upgraded to handle high pressure and thermal shock loading beyond the present scope of the contract. Present design is capable of withstanding cryogenic thermal shock and full scale static test pressures. Combustion thermal conditions, as they would affect the mounting boss area, have not yet been considered. Multiple chevron (metal, teflon, metal) or K-seals are recommended for testing. Special sizes are required.

3.1.3 Diaphragm burnout conditions should be considered, and escape of combustion gases should be restricted. Multiple internal pressure baffling and possible threaded cable cap construction should be reviewed.

3.2 Four-active-element Silicon Chip Beam

3.2.1 Change in electrical resistance of the individual elements of the silicon chip beam with from zero to full scale distributed pressure on the diaphragm indicates that the compression gages (position 2 and 4) (see Table 2, Appendix III) are contributing only a small amount in the way of output. It should be possible, without overdriving the diaphragm, to redesign the silicon chip to increase the full scale output to at least 100 mv. Increased output would: (1) decrease the L-H and R error band and (2) decrease thermal effects (sensitivity change and zero drift). Also further geometrical changes in the gage layout should be investigated to enhance the output and reduce the normal bridge electrical imbalance.

3.3 Thermal Environment: Transient and Steady State

3.3.1 By submerging the transducer completely in cryogenic fluid to a depth beyond the cable cap (see Fig. 6), thermal equilibrium is quickly achieved, both in the diaphragm area as well as in the electrical bridge compensation area. If both areas are not at identical temperatures nor achieve it simultaneously, transient thermal output could be large and the electrical compensation for thermal effects either slow to stabilize or never quite achieved. To achieve fast stability, submersion technique was employed. In terms of field (or flight) tests, this latter procedure is probably unrealistic. Relocation of the passive compensation elements to the liquid cooled region of the transducer is desirable.

3.3.2 To achieve a realistic thermal environment error band of ΔS and ΔZ for the PT15C-2, testing over the entire cryogenic temperature range is believed necessary. Tests were conducted at LN_2 and LH_2 ; however, ambiguities in the results (see calibration sheets) indicate a need for further investigation in this area. The problem here is probably related to the passive compensating components used in the three subject transducers. Further component testing should correct this situation.

4. CONCLUSION

Modification to Electro-Optical Systems' novel combustion pressure transducer^{*}, commercially available in two sizes, the PT15C-3 for a minimal access geometry problem, and PT15B-2 (Figs. 11, 12, and 13) for insertion in an AND 10050-4 boss geometry, such that it could be cooled by LH_2 , has resulted in a useful first generation device.

The results prove the feasibility of the use of a solid state silicon four-active-arm piezoresistive element, arranged as a Wheatstone bridge, over a large temperature span, 20°K to $> 300^\circ\text{K}$, with good output for direct recording and within a transducer geometry utilizing the sensor's inherent small size, fast thermal response, and linear characteristics. These transducers, identified as model PT15C-2, can provide the electromechanical means for measuring static (0 to 1500 psig) and dynamic (flat dc to 10 kc) pressures under combustion environment, flush within a liquid rocket cryogenic-cooled motor.

^{*} Patent pending

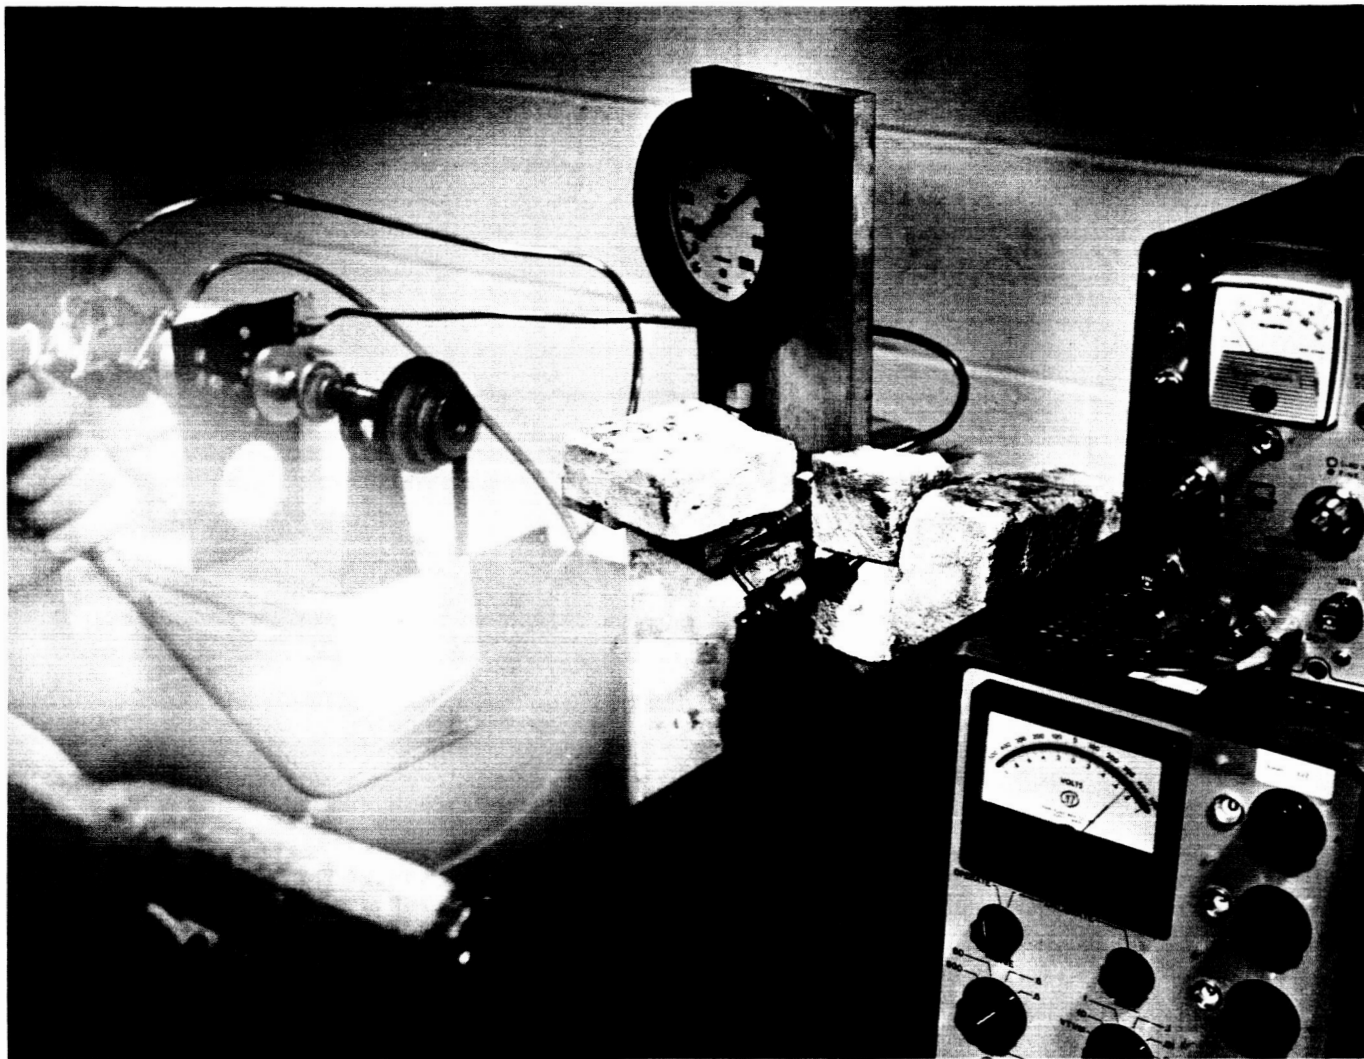


FIG. 11 EOS DEVELOPED PT15B COMBUSTION PRESSURE TRANSDUCER WITH COOLANT FLOW
IN OPERATION JUST PRIOR TO FLAME IMPINGEMENT

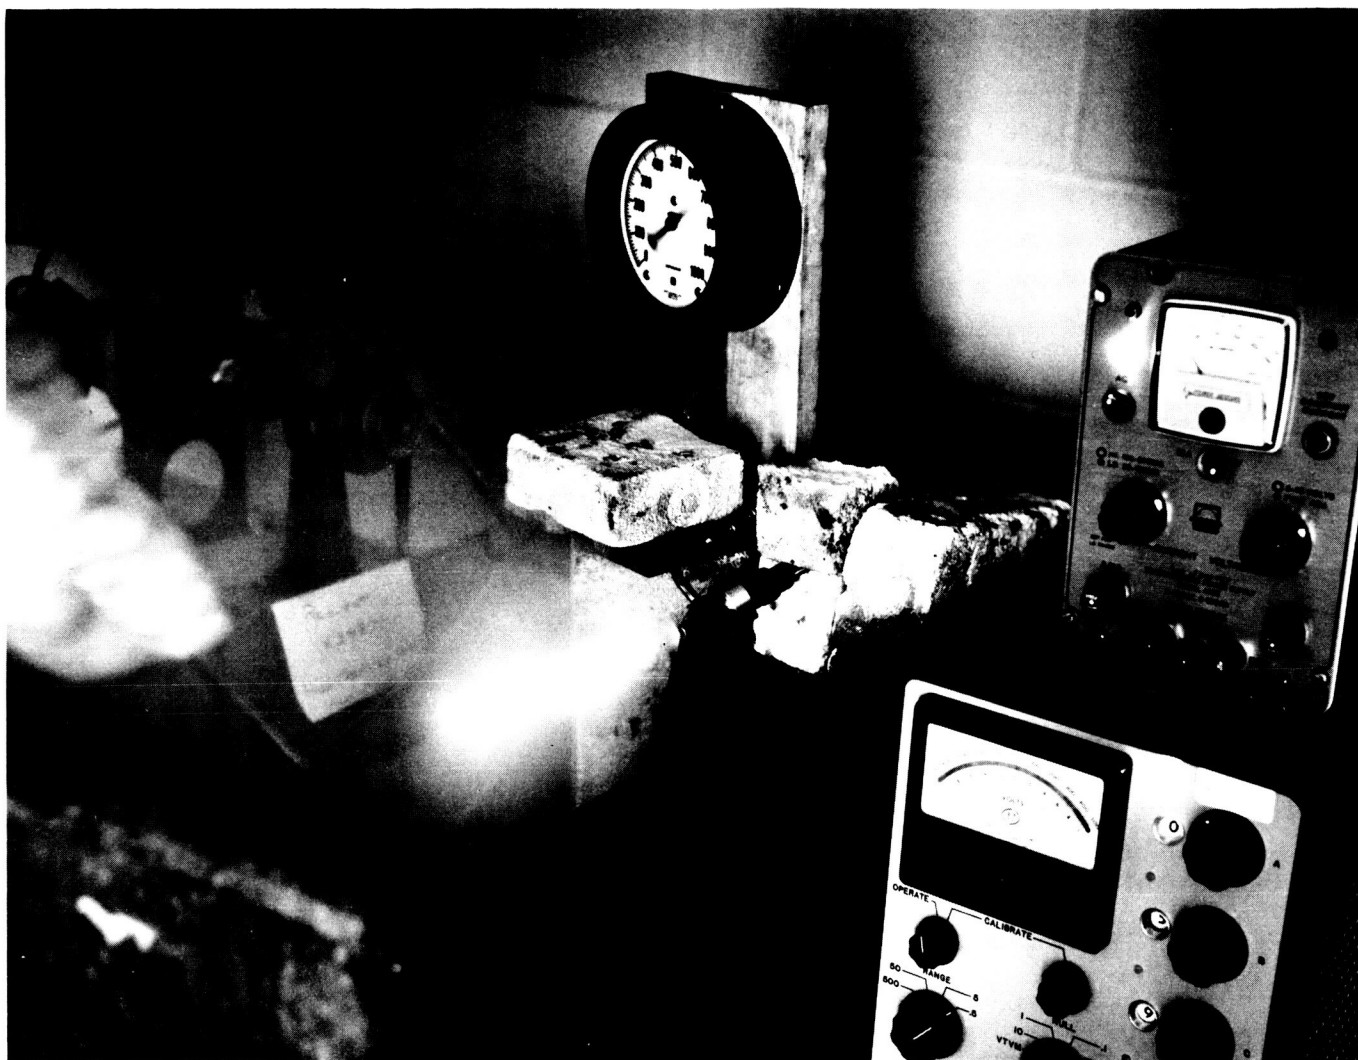


FIG. 12 OXY-HYDROGEN FLAME IMPINGEMENT DIRECTLY ON DIAPHRAGM
OF PT15B COMBUSTION PRESSURE TRANSDUCER

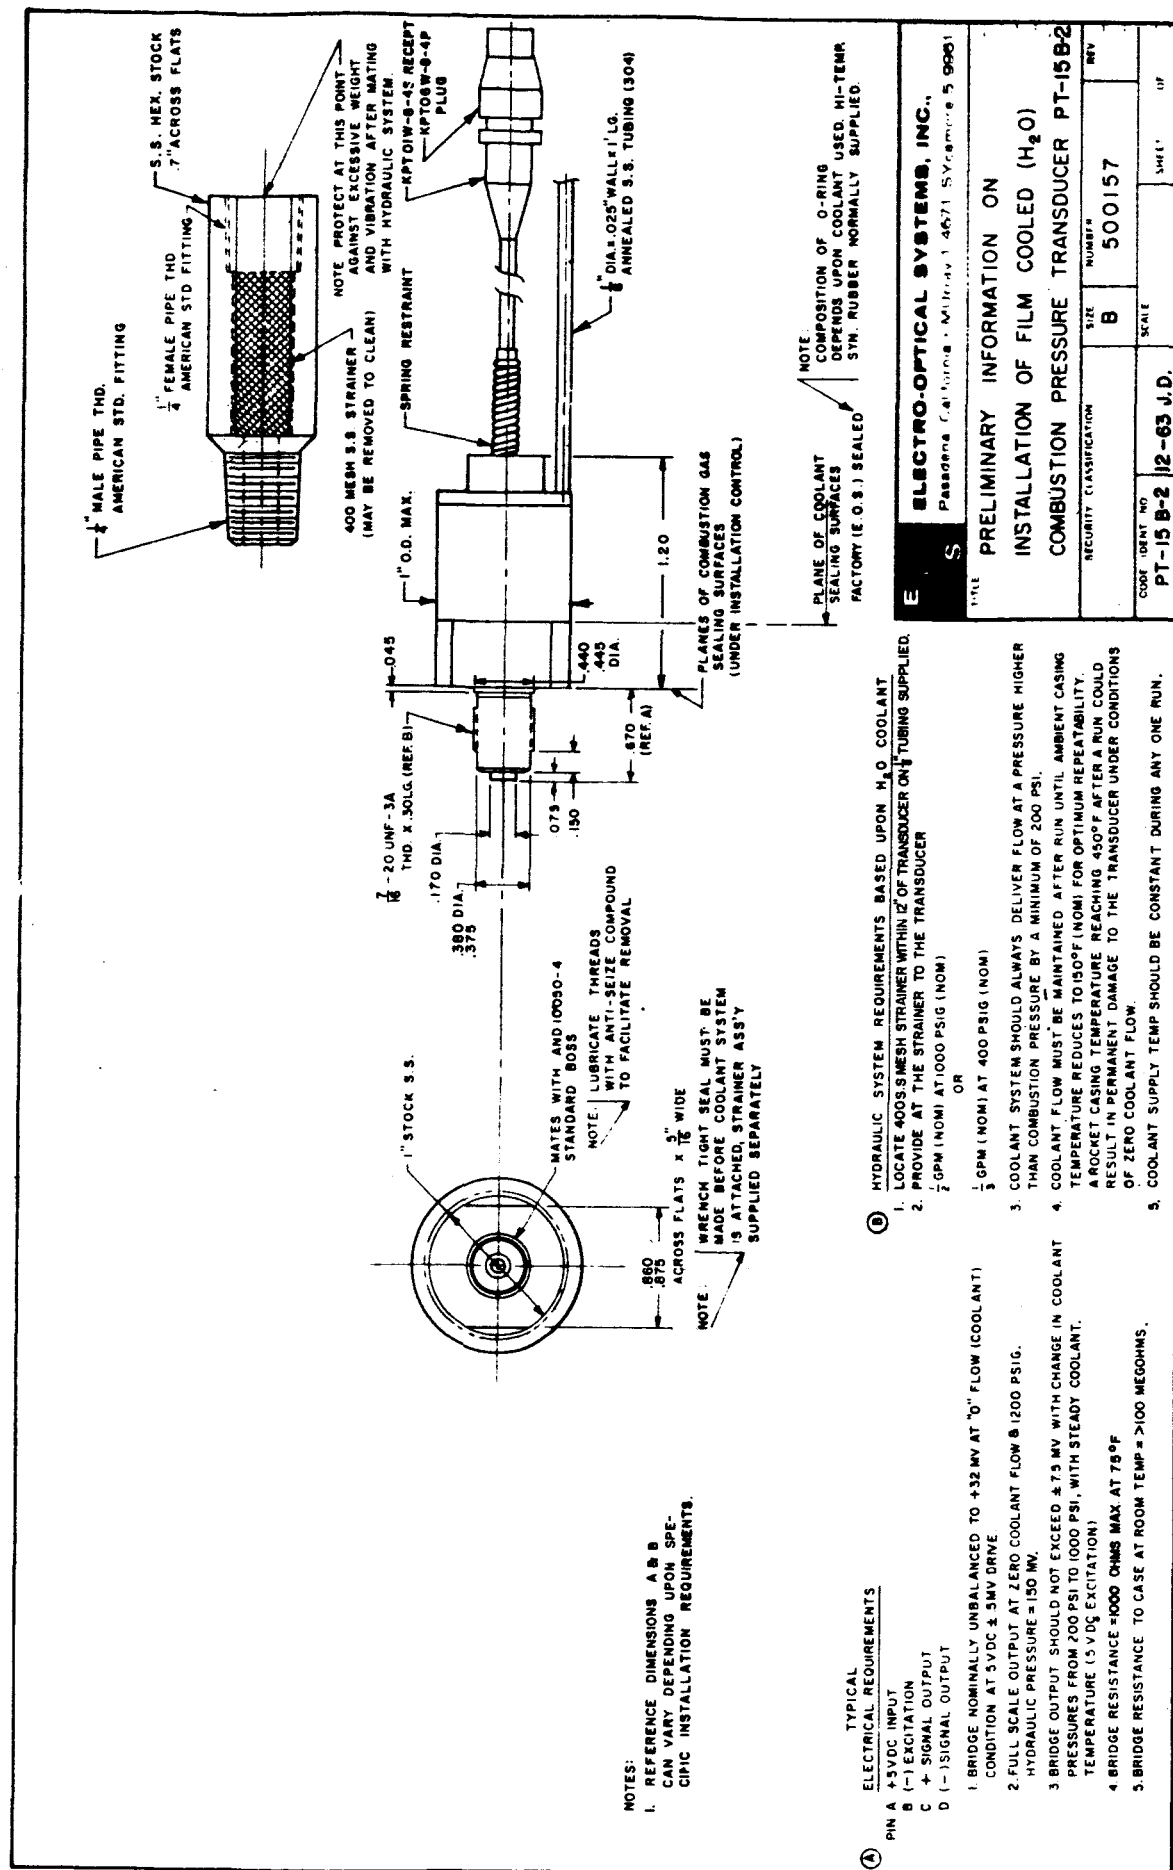


FIG. 13 PRELIMINARY INFORMATION ON INSTALLATION OF FILM COOLED (H₂O) COMBUSTION PRESSURE TRANSDUCER PT15B-2

APPENDIX I
LIST OF ABBREVIATIONS

APPENDIX I

List of Abbreviations

T'N	=	tension gage
C'N	=	compression gage
TCB	=	thermo-compression bonded
F.S.	=	full scale
S	=	sensitivity (output over the full scale pressure range)
RT	=	room temperature
S _{RT}	=	sensitivity at room temperature
ΔS	=	change in full scale output over temperature range
Z	=	zero balance of the transducer electrical bridge
ΔZ	=	change of zero balance over temperature range
R	=	resistance
ΔR	=	change of resistance
V	=	voltage (dc)
T	=	temperature $\frac{\Delta R}{R}$
G.F.	=	gage factor = $\frac{R}{\epsilon}$
ε	=	strain, inches per inch
μ	=	micro, one millionth
Ω	=	ohms
UP	=	increasing pressure steps (as during a calibration run)
DN	=	decreasing pressure steps (as during a calibration run)
E _O	=	voltage output
E _{IN}	=	voltage input
I = K	=	constant current
V = K	=	constant voltage
L-H & R	=	combined accuracy; linearity, hysteresis, and repeatability
SS	=	stainless steel

APPENDIX II
FABRICATION OF SINGLE CHIP BEAMS IN SILICON,
HAVING FOUR-ACTIVE STRAIN GAGE ARMS

Author: Stephen Kaye

FABRICATION OF SINGLE CHIP BEAMS IN SILICON,
HAVING FOUR-ACTIVE STRAIN GAGE ARMS

S. Kaye

1. Design

The design of the silicon diaphragm for use in pressure measurements, where the silicon is intended to be bonded to a clamped metal diaphragm of 60 mils diameter, was undertaken.

It was decided to use a diffused construction where the gages were p-type diffused into an n-type 20 ohm cm silicon substrate. The substrate material selected had a [110] orientation and gages, each of which has an active area of 10 x 1 mils, were oriented with their long dimensions parallel to the [110] direction lying in the plane of the slice. In this way the strain transverse to the gage was in a [100] direction where the piezoresistive coefficient is negligible (Ref. 1).

O. N. Tufte and E. L. Stelzer (Ref. 2) have shown that the piezoresistive properties of a diffused layer are characterized by the surface concentration, once a particular distribution of impurities is assumed. Their data, which assures complementary error function distribution of impurities, was used in estimating the gage factor.

Since the gages are designed to work down to 20°K, it was necessary to select a surface concentration sufficiently large that the gage resistance would not vary significantly over the temperature range of interest.

From Morin and Maita's data (Ref. 3), it appears that p-type material, having boron concentrations in excess of 1.5×10^{19} atoms/C.C. has a resistivity almost independent of temperature in the range of 15°-300°K. It was decided, therefore, to aim for a surface concentration of 10^{20} atoms/C.C.

Ref. 1 - O. N. Tufte, et al., "Silicon Diffused Element Piezoresistive Diaphragms"; J.A.P. Vol. 33, p. 3322, November 1962

Ref. 2 - O. N. Tufte and E. L. Stelzer, "Piezoresistive Properties of Diffused Silicon Layers," J.A.P. Vol. 34, p. 313, February 1963

Ref. 3 - F. J. Morin and J. P. Maita, Phys. Rev., Vol. 96, p. 28, October 1, 1962

Under the diffusion conditions used, it was expected that a gaussian distribution of impurities would result. It was decided to use a 1μ junction depth. Using Irvin's data (Ref. 4), it was found that this would give a sheet resistance of 40 ohms/square, and hence a gage resistance of 400 ohms per element.

Using the curves in Ref. 1, a gage factor of 65 was predicted. Values were also calculated for a surface concentration of 5×10^{19} . This gave a gage resistance of 800 ohms/square, and a gage factor of 75.

The stress distribution expected in a clamped diaphragm is such that it is desirable to place two gages close to the center of the diaphragm where they will be in tension, and two close to the edge where they will be in compression. It was decided to make each element 10 mils x 1 mil, and the configuration shown in Fig. 2 of the main text of this report was used. In order to avoid unwanted stiffening of the diaphragm by soldered contacts, it was decided to use 1 micron of aluminum evaporated and alloyed to form ohmic contacts to the active elements, and then attach external leads by bonding or welding to contact pads placed on approximately the neutral axis of the diaphragm.

2. Fabrication Techniques

Table I lists the major process steps in the fabrication of the silicon chips.

Steps 1-27 are carried out on complete slices each having approximately 60 units. Steps 28 and 29 are on individual units.

Ref. 4 - J. C. Irvin, "Resistivity of Bulk Silicon and of Diffused Layers in Silicon," B.S.J.T., Vol. XLI, p. 387, March 1962

TABLE I

1. Procure silicon - 20 ohm cm n-type [110] orientation with (100) face marked by a flat ground on one edge. Slices 1" $\pm 1/8$ diameter, .010" thick.
2. Polish etch - remove approximately 2 mils.
3. Oxidize - 1200°C 2 hours, wet oxygen.
4. Coat with photoresist and align mesa pattern with (100) edge.
5. Expose, develop, and bake resist.
6. Etch mesas - approximately 1 mil deep.
7. Remove photoresist, clean, slice, and remove oxide.
8. Reoxidize - 1200°C 1 hour, wet oxygen.
9. Coat with photoresist and register gage pattern.
10. Expose, develop, and bake resist.
11. Etch oxide.
12. Remove resist and clean slice.
13. Predeposit boron - 1050°C 20 minutes
 B_2O_3 source
14. Drive in - 1050°C 30 minutes.
15. Coat with photoresist and register contact pattern.
16. Expose, develop, and bake resist.
17. Etch oxide.
18. Remove resist and clean slice.
19. Check gage resistance.
20. Evaporate aluminum - 1 μ thick.
21. Coat with photoresist and register inverted contact pattern.

22. Expose, develop, and bake resist.
23. Etch aluminum.
24. Alloy aluminum.
25. Check gage resistance.
26. Mount for etching face down.
27. Etch back of slice to separate and reduce gage thickness to .0005".
28. Demount, clean, and visual inspect.
29. Bond leads.

APPENDIX III

TABLES

- 1 R versus T
- 2 304 Data
Invar Data
- 3 NiSpan C Diaphragms
- 4 Calibration Data
(Series 2, 3 and 4)

Table 1

	T °K	<u>Unbonded</u>			<u>Bonded to 304 SS</u>	
		<u>S-G 4B Gage</u>	<u>S-G 4B Gage</u>		<u>S-G 4B Gage</u>	<u>S-G 4B Gage</u>
		<u>Compression Gage</u>	<u>Tension Gage</u>		<u>Compression Gage</u>	<u>Tension Gage</u>
	296	498.8Ω	460.1Ω	(EOS)	488.3Ω	390.0Ω
LN ₂	77	390.3	356.5	↑	343.7	256.5
LO ₂	90				348.7	259.8
CO ₂	195	443.4	407.7		411.4	312.0
	296	499.2	460.6		489.3	391.0
	77	390.3	356.6		343.7	256.5
	90				348.7	299.8
CO ₂	195	443.0	407.4		411.3	311.9
	296	499.2	461.2	(EOS)	488.3	389.9
	300	500.7	462.4	(Wyle Lab)	491.0	392.3
LH ₂	20	372.7	340.2	↑	329.7	247.4
	300	499.1	462.8		492.4	393.7
	20	372.7	341.1		329.9	247.4
	300	500.6	465.2		492.9	394.2
	20	372.9	342.3		330.0	247.5
	300	502.4	466.8		495.1	396.3
	20	372.8	342.5		330.1	247.6
	300	501.9	466.8		494.7	396.6
	20	373.0	342.7		330.1	247.5
	300	503.6	468.8	(Wyle Lab)	495.7	396.8
	297	500.0	465.3	(EOS)	491.4	392.6
Boil H ₂ O	370			(EOS)	552.1	454.0
	297			(EOS)	491.4	392.7

Typical resistance readings of individual elements of a silicon beam chip vs. temperature as read by the wheatstone bridge method; 1-1/2 VDC power.

Table 2

Typical bonded silicon chip, individual element resistance changes with temperature:

I 304 S.S. Diaphragm

T, °K	R, Ω	R, Ω	R, Ω	R, Ω
297	415.7	533.0	430.0	486.7
77	270.6	374.0	279.2	337.5
297	414.7	531.9	429.1	485.7
77	270.7	374.1	279.2	337.3
297	416.0	533.0	430.1	486.4
297	414.2	531.8	428.8	485.4


II Invar Steel Diaphragms

Typical bonded resistance change with temperature:

T, °K	R, Ω	R, Ω	R, Ω	R, Ω	R, Ω	R, Ω
297	471.1	597.4	474.1	503.8	468.4	559.8
77	359.3	464.3	362.2	387.0	359.5	440.2
297	469.5	595.6				
195	416.5	531.7				

All the above resistance elements were pressure cycled while at the indicated temperature.

III Typical resistance changes with temperature before and after bonding to Invar constant stress beam and when strained to 1000 microinches.

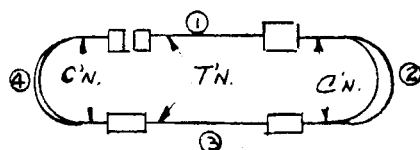


Data S=K=Beam

Gage #25 S.G. 6C - Aluminum thermal compression bonded leads

T, °K	Step 250 μ in. strain	①	②	③	④	
297		419.9	537.5	429.8	476.9	Unbonded
77		327.3	419.0	333.1	371.8	"
297	0	405.8	516.0	415.7	465.8	Bonded to
	1	410.8	519.0	420.8	469.1	Invar constant
	2	415.8	522.0	425.7	472.3	stress beam
	3	420.9	525.1	430.9	475.8	
	4	426.1	528.1	436.1	479.1	
77	0	282.3	377.5	287.4	337.3	0 microstrain "/"
	1	286.7	381.0	291.9	340.9	250 "
	2	291.2	384.5	296.5	344.7	500 "
	3	296.3	388.3	301.7	348.8	750 "
	4	302.0	392.4	307.4	353.3	1000 "

Table 3

Unbonded and bonded resistance of actual 4-element silicon beam chips on NiSpan C diaphragms used in PT15C-2 transducers:

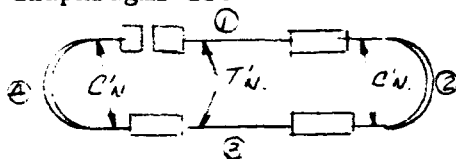

4-element silicon chip
.040" x .060"

<u>Gage No.:</u>	<u>①</u>	<u>②</u>	<u>③</u>	<u>④</u>	<u>Method</u>
<u>Unit #2</u>					
Unbonded @ RT	463.5 Ω	515.9 Ω	467.4 Ω	564.9 Ω :	Wheatstone bridge, 1.5v excitation
Bonded* 0 PSIG	457.0 Ω	495.0 Ω	458.0 Ω	541.0 Ω :	Oil dead weight tester and Wheat- stone bridge network 5 VDC excit.
at R.T. 1500 PSIG	476.0	492.0	477.0	537.0	
ΔR	+ 19.0	- 3.0	+ 19.0	- 2.3	
Element #12					
<u>Unit #3</u>					
Unbonded at RT	485.0 Ω	604.1 Ω	484.1 Ω	553.9 Ω	Wheatstone bridge, 1.5V excitation
Bonded* 0 PSIG	480.0 Ω	583.0 Ω	495.0 Ω	523.0 Ω	Oil dead weight tester and Wheat- stone bridge net- work 5 VDC excit.
at R.T. 1500 PSIG	497.0	583.0	514.0	520.0	
ΔR	+ 17.0	0	19.0	- 3.0	
Element #5					
<u>Unit #4</u>					
Unbonded* @ R.T.	438.3 Ω	524.3 Ω	449.9 Ω	564.5 Ω	Wheatstone bridge, 1.5v excitation
Bonded* 0 PSIG	426.0 Ω	519.0 Ω	437.0 Ω	533.0 Ω	Oil dead weight tester and Wheat- stone bridge network 5 VDC excitation
at R.T. 1500 PSIG	443.0	517.0	453.0	529.0	
ΔR	+ 17.0	- 2.0	+ 16.0	- 4.0	
Element #9					

*To NiSpan C material diaphragm.

Table 4

CALIBRATION TEST DATA

PT15C-2 Serial #3				PT15C-2 Serial #2		PT15C-2 Serial #4	
T	Pressure PSIG	E _O Up	E _O Dn.	E _O Up	E _O Dn.	E _O Up	E _O Dn.
RT	0	+25.2 mv	25.0 mv	24.6 mv	23.2 mv	+16.1 mv	14.6 mv
75°F	250	36.5	34.0	38.0	36.0	27.4	26.0
	500	47.9	45.4	51.4	49.5	38.8	37.4
(EOS)	750	59.4	56.8	65.1	63.9	50.4	49.2
	1000	71.0	68.9	78.5	77.3	62.3	61.5
	1250	82.6	81.2	92.8	91.8	74.4	73.6
	1500	94.6		107.1		86.5	
	SRT=69.4mv at I=K=10 MA			SRT=82.5 at I=K=10 MA		SRT=70.4 at I=K=12 MA	
LN ₂	0	+13.3	14.3	+10.6	10.2	+ 4.6	+ 4.6
	250	24.7	25.3	23.0	23.0	14.7	14.4
	500	35.7	36.8	36.2	36.1	23.7	23.7
(EOS)	750	47.9	48.3	49.5	49.4	34.9	34.8
	1000	60.0	60.5	63.5	63.4	46.2	46.0
	1250	73.0	73.0	77.5	77.5	58.0	57.7
	1500	86.5		92.8		70.1	
	SLN ₂ =73.2mv at I=K=10 MA			SLN ₂ = 82.2 at 10 MA		SLN ₂ = 65.5 at 12 MA	
RT	0 psig	23.6 mvDC		RT 0	+30.5	RT 0	+12.7
	1500 psig	97.6 mvDC		1500	116.4	1500	83.2
(Norco)	0 psig	23.6 mvDC		0	30.5	0	11.7
	0	+ 6.0	6.0	(23.4)	23.7	29.0	29.0
	250	15.6	15.6	35.4	35.6	39.1	39.3
	500	27.7	25.7	47.5	47.3	49.5	47.2
LH ₂	750	36.1	36.1	60.0	60.1	59.8	57.8
(Norco)	1000	47.0	47.0	73.3	72.6	70.5	70.6
	1250	58.5	58.5	86.8	86.3	81.8	80.6
	1500	70.3		100.3		93.1	
	SLH ₂ =64.3 mv at I=K=10 MA			*SLH ₂ =76.6 mv at 10 MA		SLH ₂ =64.1 mv at 12 MA	
(EOS)	0 psig	22.6 mvDC		0 psig	30.8 mvDC	0 psig	11.4 mvDC
RT	1500 psig	96.6 mvDC		1500 psig	112.3 mvDC	1500 psig	82.0 mvDC
	0 psig	22.2 mvDC		0 psig	30.8 mvDC	0 psig	10.5 mvDC
RT to LN ₂ RT to LH ₂				RT to LN ₂ RT to LH ₂		RT to LN ₂ RT to LH ₂	
Δ Zero Shift % FS/100°F				- 4.28 - 1.585		- 4.13 + 4.63	
Δ Sensitivity Change: +1.385 - 2.62 % FS/100°F				- .0922 - 2.17		- 1.76 - 1.82	
Effect of Mass Coolant Flow on Zero Balance, H ₂ O at 650 psi=.2mv I=K=10 MA				.2mv I=K=10 MA		.3mv I=K=12 MA	
Weight = 85 gms.				85 gms.		85 gms.	
Final Bridge Resistances:							
Output A-B 560Ω				540Ω		570Ω	
Input D-C 435				420		365	
D-A 360				350		380	
D-B 420				400		440	

III-4

*Several runs made.

APPENDIX IV
PT15C-2 PARTS LIST

ENGINEERING PARTS LIST

ENGINEERING PARTS				DESCRIPTION				
ITEM NO.	DWG NO.	PART NO.	REV.	REQ'D. PER ASSEMBLY				DESCRIPTION
1	D	427021		1			/	Pressure Transducer Model PT15C-2
2				1				Hex Blast Tube Assembly
3	C	612732-2			1			Blast Tube, Hex
4	C	4270010			1			Plate, Deflector
5					AR			Silver Solder
6								
7								
8				1				Instrument Housing Assembly
9	D	612733-2			1			Housing, Instrument
10		427019			1			Tube, Coolant
11					AR			Silver Solder
12								
13								
14		427018			1			Diaphragm Assembly
15					1			Anchor Assembly
16	C	4771001				1		Diaphragm
17	C	4771002				1		Anchor, Diaphragm
18						AR		Silver Solder
APPROVED								
NEXT ASSEMBLY				DWG NO. 427021		COMPILED BY		PAGE 1 OF 4
TITLE				None		R. Pycs		P/L 427021
EOS ELECTRO OPTICAL SYSTEMS INC.				ASSY. TITLE		Pressure Transducer Model PT15C-2		

ENGINEERING PARTS LIST

ITEM NO	DWG NO	PART NO.	REV.	REQ'D. PER ASSEMBLY										DESCRIPTION	
19															Harness and Strain Gage Assembly
20		427016									1				Silicon Strain Gage Assembly
21		427013										1			Silicon Strain Gage Chip
22													AR		Wire, Aluminum (.001 Dia.)
23		427015									1				Strain Gage Wire Harness
24													5		Insulated Magnet Wire (.003 dia. x 3")
25												AR			Solder (SN 95% AG 5%)
26															
27											AR				Cement (Furane x 5B)
28		427017									1				Harness Support Block
29											AR				Cement, Epoxy No. 502
30		427014										1			Seal (Gold)
31															
32										8					Solder Tab
33											AR				Solder (SN 95% AG 5%)
34															
35															
36															
APPROVED															
NEXT ASSEMBLY TITLE		None		DWG NO.		427021		COMPILED BY		R. Pycz		PAGE 2		OF 4	
EOS ELECTRO OPTICAL SYSTEMS INC.				ASSY. TITLE		Pressure Transducer Model PT15C-2		P/L		427021					

ENGINEERING PARTS LIST

ITEM NO.	DWG NO.	PART NO.	REV.	REQ'D. PER ASSEMBLY	DESCRIPTION
37	C	4771011		1	Cable Assembly
38	C	4771007		1	Cap. Cable
39	C	4771008		1	Insulator, Cable
40	B	4771014		1	Spring
41				1	Set screw, Hex Hd. No. 0-80 x 1/8 Cup Point
42				1	Connector (Cannon KPT06F8-4P or equiv.)
43			AR		Solder (SN-60)
44			AR		Epoxy - Clear
45			AR		Catalyst
46	B	4771009		1	Cable
47					
48					
49		427020		1	O-Ring, Metal
50				4	Screw, Machine-Hex Hd. No. 2-56 x 1/4
51				3	Screw, Machine-Hex Hd. No. 2-56 x 1/2
52				1	Resistor (Sensitivity)
53				1	Resistor (Balance)
54				1	Resistor (Zero Shift)
APPROVED					
NEXT ASSEMBLY		None	DWG NO. 427021		COMPILED BY R. Pycz
E.O.S. ELECTRO OPTICAL SYSTEMS INC.			ASSY. TITLE Pressure Transducer PT 15G-2		PAGE 3 OF 4
					P/L 427021

ENGINEERING PARTS LIST

ITEM/DWG NO. SIZE	PART NO.	REV.	REQ'D. PER ASSEMBLY	DESCRIPTION
55			AR	Wire Copper (.004 dia.)
56				
57			AR	Solder SN 95% AG 5%
58			1	Dust Cap
59			1	Dust Cap
60			1	Dust Cap
61			AR	Sleeving
62			AR	Cement (Furane x 5B)
63				
64				
65			1	Connector (Cannon KPT00 P-8-4S or Equiv.)
66				
67				
68				
69				
70				
71				
72				
APPROVED				
NEXT ASSEMBLY			DWG NO.	COMPILED BY
TITLE			None	R. Pycz
E.O. ELECTRO OPTICAL SYSTEMS INC.			ASSY. TITLE	P/L 427021
				PAGE 4 OF 4

DISTRIBUTION LIST FOR FINAL REPORT

Contract NAS3-2754

"Liquid Hydrogen Film Cooled Pressure Transducer"

Electro-Optical Systems, Inc.

Report is to be sent directly to the "Recipients" marked with an "X" under the column headed "Designee" on Pages 1 and 2 only. On Pages 3 through 10, the report should be sent to the Technical Librarian of the "Recipient" with a carbon copy of the letter of transmittal to the attention of the person named under the column "Designee". The letter of transmittal should contain the contract number and complete title of the final report.

The distribution list should be included in the final report as an appendix.

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	NASA Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135 Attn: Office of Technical Information	(X)
1	NASA Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135 Attn: Contracting Officer	(X)
1	NASA Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135 Attn: Patent Office	(X)
4	NASA Headquarters Washington, D. C. 20546 Attn: Mr. Henry Burlage, Jr. Chief, Liquid Propulsion Systems, RPL	(X)
1	NASA Headquarters Washington, D. C. 20546 Attn: Mr. Vernon E. Jaramillo Advanced Manned Mission, MTC	(X)

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
25	Scientific and Technical Information Facility NASA Representative, Code CRT P. O. Box 5700 Bethesda, Maryland 20014	(X)
1	NASA Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135 Attn: Mr. James W. Norris Mail Stop 500-305	(X)
1	NASA Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135 Attn: Mr. Gerald Morrell	(X)
1	NASA Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135 Attn: Mr. R. J. Crowl	(X)
1	NASA Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135 Attn: Mr. C. C. Gettelman	(X)

N A S A F I E L D C E N T E R S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
2	Ames Research Center Moffett Field, California 94035	Harold Hornby Missions Analysis Division
2	Goddard Space Flight Center Greenbelt, Maryland 20771	Merland L. Moseson Code 623
2	Jet Propulsion Laboratory Calif. Institute of Technology 4800 Oak Grove Drive Pasadena, California 91103	Robert F. Rose Propulsion Div., 38
2	Langley Research Center Langley Station Hampton, Virginia 23365	Floyd L. Thompson Director
2	Lewis Research Center 21000 Brookpark Road Cleveland, Ohio 44135	Dr. Abe Silverstein Director
2	Marshall Space Flight Center Huntsville, Alabama 35812	Hermann K. Weidner Code R-P&VED
2	Manned Spacecraft Center Houston, Texas 77001	Robert R. Gilruth Director
2	Western Operations Office 150 Pico Boulevard Santa Monica, California 90406	Robert W. Kamm Director

G O V E R N M E N T I N S T A L L A T I O N S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	Advanced Research Projects Agency Washington 25, D. C.	D. E. Mock
1	Aeronautical Systems Division Air Force Systems Command Wright-Patterson Air Force Base Dayton, Ohio 45433	D. L. Schmidt Code ASRCNC-2
1	Air Force Missile Development Center Holloman Air Force Base, New Mexico	Maj. R. E. Bracken Code MDGRT
1	Air Force Missile Test Center Patrick Air Force Base, Florida	L. J. Ullian
1	Air Force Systems Command, Dyna-Soar Air Force Unit Post Office Los Angeles 45, California	Col. Clark Technical Data Center
1	Arnold Engineering Development Center Arnold Air Force Station Tullahoma, Tennessee	Dr. H. K. Doetsch
1	Bureau of Naval Weapons Department of the Navy Washington 25, D. C.	J. Kay, Code RTMS-41
1	Defense Documentation Center Headquarters Cameron Station, Building 5 5010 Duke Street Alexandria, Virginia 22314 Attn: TISIA	
1	Headquarters, U. S. Air Force Washington 25, D. C.	Col. C. K. Stambaugh Code AFRST
1	Picatinny Arsenal Dover, New Jersey 07801	I. Forsten, Chief Liquid Propulsion Laboratory
1	Rocket Research Laboratories Edwards Air Force Base Edwards, California 93523	Colonel Silk

G O V E R N M E N T I N S T A L L A T I O N S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	U. S. Atomic Energy Commission Technical Information Services Box 62 Oak Ridge, Tennessee	
1	U. S. Army Missile Command Redstone Arsenal, Alabama 35809	Dr. Walter Wharton
1	U. S. Naval Ordnance Test Station China Lake, California 93557	Code 451 Chief, Missile Propulsion Division

C P I A

1	Chemical Propulsion Information Agency Johns Hopkins University Applied Physics Laboratory 8621 Georgia Avenue Silver Spring, Maryland	Neil Safeer
---	--	-------------

C O M M E R C I A L C O N T R A C T O R S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	Aerojet-General Corporation P. O. Box 296 Azusa, California	L. F. Kohrs
1	Aerojet-General Corporation P. O. Box Box 1947 Technical Library, Bldg 2015, Dept. 2410 Sacramento, 9, California 95809	R. Stiff
1	Aerojet-General Corporation P. O. Box 1947 Technical Library, Bldg. 2015, Dept. 2410 Sacramento, California 95809	R. D. Wesley
1	Aeronutronic A Division of Ford Motor Company Ford Road Newport Beach, California	D. A. Carrison
1	Aerospace Corporation 2400 East El Segundo Boulevard P. O. Box 95085 Los Angeles, California 90045	John G. Wilder MS-2293 Propulsion Dept.
1	Arthur D. Little, Inc. Acorn Park Cambridge 40, Massachusetts	A. C. Tobey
1	Astropower, Inc., Subsidiary of Douglas Aircraft Company 2968 Randolph Avenue Costa Mesa, California	Dr. George Moc Director, Research
1	Astrosystems, Inc. 1275 Bloomfield Avenue Caldwell Township, New Jersey	A. Mendenhall
1	Atlantic Research Corporation Edsall Road and Shirley Highway Alexandria, Virginia	A. Scurlock
1	Beech Aircraft Corporation Boulder Facility Box 631 Boulder, Colorado	J. H. Rodgers

C O M M E R C I A L C O N T R A C T O R S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	Bell Aerosystems Company P. O. Box 1 Buffalo 5, New York	W. M. Smith
1	Bendix Systems Division Bendix Corporation Ann Arbor, Michigan	John M. Brueger
1	Boeing Company P. O. Box 3707 Seattle 24, Washington	J. D. Alexander
1	Chrysler Corporation Missile Division Warren, Michigan	John Gates
1	Curtiss-Wright Corporation Wright Aeronautical Division Woodridge, New Jersey	G. Kelley
1	Douglas Aircraft Company, Inc. Missile and Space Systems Division 3000 Ocean Park Boulevard Santa Monica, California 90406	R. W. Hallet Chief Engineer Advanced Space Tech.
1	Fairchild Stratos Corporation Aircraft Missiles Division Hagerstown, Maryland	J. S. Kerr
1	General Dynamics/Astronautics Library & Information Services (128-00) P. O. Box 1128 San Diego, California 92112	Frank Dore
1	General Electric Company Re-Entry Systems Department Box 8555 Philadelphia, Pennsylvania 19101	F. E. Schultz
1	General Electric Company Flight Propulsion Lab Department Cincinnati 15, Ohio	D. Suichu

C O M M E R C I A L C O N T R A C T O R S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	Grumman Aircraft Engineering Corp. Bethpage Long Island, New York	Joseph Gavin
1	Kidde Aero-Space Division Walter Kidde and Company, Inc. 675 Main Street Belleville 9, New Jersey	R. J. Hanville Director of Research Engineering
1	Lockheed California Company 10445 Glen Oaks Boulevard Pacoima, California	G. D. Brewer
1	Lockheed Missiles and Space Company Attn: Technical Information Center P. O. Box 504 Sunnyvale, California	Y. C. Lee Power Systems R&D
1	Lockheed Propulsion Company P. O. Box 111 Redlands, California	H. L. Thackwell
1	The Marquardt Corporation 16555 Saticoy Street Box 2013 - South Annex Van Nuys, California 91409	Warren P. Boardman, Jr.
1	Martin Division Martin Marietta Corporation Baltimore 3, Maryland	John Calathes (3214)
1	Martin Denver Division Martin Marietta Corporation Denver, Colorado 80201	J. D. Goodlette Mail A-241
1	McDonnell Aircraft Corporation P. O. Box 6101 Lambert Field, Missouri	R. A. Herzmark
1	North American Aviation, Inc. Space & Information Systems Division Downey, California	H. Storms

C O M M E R C I A L C O N T R A C T O R S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	Northrop Corporation 1001 East Broadway Hawthorne, California	W. E. Gasich
1	Pratt & Whitney Aircraft Corp. Florida Research and Development Center P. O. Box 2691 West Palm Beach, Florida 33402	R. J. Coar
1	Radio Corporation of America Astro-Electronics Division Defense Electronic Products Princeton, New Jersey	S. Fairweather
1	Reaction Motors Division Thiokol Chemical Corporation Denville, New Jersey 07832	Arthur Sherman
1	Republic Aviation Corporation Farmingdale, Long Island, New York	Dr. William O'Donnell
1	Rocketdyne (Library Dept. 586-306) Division of North American Aviation 6633 Canoga Avenue Canoga Park, California 91304	E. B. Monteath
1	Space General Corporation 9200 Flair Avenue El Monte, California	C. E. Roth
1	Space Technology Laboratories Subsidiary of Thompson-Ramo-Wooldridge P. O. Box 95001 Los Angeles 45, California	G. W. Elverum
1	Stanford Research Institute 333 Ravenswood Avenue Menlo Park, California 94025	Thor Smith
1	TAPCO Division Thompson-Ramo-Wooldridge, Inc. 23555 Euclid Avenue Cleveland 17, Ohio	P. T. Angell

C O M M E R C I A L C O N T R A C T O R S

<u>COPIES</u>	<u>RECIPIENT</u>	<u>DESIGNEE</u>
1	Thiokol Chemical Corporation Redstone Division Huntsville, Alabama	John Goodloe
1	United Aircraft Corporation Research Laboratories 400 Main Street East Hartford, Connecticut 06108	Erle Martin
1	United Technology Center 587 Methilda Avenue P. O. Box 358 Sunnyvale, California	B. Abelman
1	Vought Astronautics Box 5907 Dallas 22, Texas	Warren C. Trent
1	Princeton University Princeton, New Jersey	D. Layton

ABSTRACT

A film cooled pressure transducer, designed for flush mounting within a rocket combustion chamber has an all silicon piezoresistive bridge network. It senses steady state pressures and has a high flat frequency response. It is capable of being cooled with liquid hydrogen, and will operate at LH_2 temperature with small change in sensitivity and bridge balance. Exposed frontal area is only 0.018 square inch.