

N 69 10 442
NASA CR 97481

SC-RR-68-592
September 1968

Research Report

CASE FILE
COPY

AN IMPROVED MODEL OF THE VACUUM PROBE

M. E. Morris, 1742, Sandia Laboratories, Albuquerque
L. W. Hughes, University of New Mexico
A. Parisi, 7214, Sandia Laboratories, Albuquerque
J. W. Beakley, University of New Mexico
W. J. Whitfield, 1742, Sandia Laboratories, Albuquerque
H. D. Sivinski, 1740, Sandia Laboratories, Albuquerque

SANDIA LABORATORIES



OPERATED FOR THE U. S. ATOMIC ENERGY COMMISSION BY SANDIA CORPORATION

ALBUQUERQUE, NEW MEXICO; LIVERMORE, CALIFORNIA

Issued by Sandia Corporation,
a prime contractor to the
United States Atomic Energy Commission

LEGAL NOTICE

This report was prepared as an account of Government sponsored work. Neither the United States, nor the Commission, nor any person acting on behalf of the Commission:

A. Makes any warranty or representation, expressed or implied, with respect to the accuracy, completeness, or usefulness of the information contained in this report, or that the use of any information, apparatus, method, or process disclosed in this report may not infringe privately owned rights; or

B. Assumes any liabilities with respect to the use of, or for damages resulting from the use of any information, apparatus, method, or process disclosed in this report.

As used in the above, "person acting on behalf of the Commission" includes any employee or contractor of the Commission, or employee of such contractor, to the extent that such employee or contractor of the Commission, or employee of such contractor prepares, disseminates, or provides access to, any information pursuant to his employment or contract with the Commission, or his employment with such contractor.

SC-RR-68-592

AN IMPROVED MODEL OF THE VACUUM PROBE*

M. E. Morris, 1742, Sandia Laboratories, Albuquerque
L. W. Hughes, University of New Mexico
A. Parisi, 7214, Sandia Laboratories, Albuquerque
J. W. Beakley, University of New Mexico
W. J. Whitfield, 1742, Sandia Laboratories, Albuquerque
H. D. Sivinski, 1740, Sandia Laboratories, Albuquerque

September 1968

ABSTRACT

The need for a microbiological surface sampling device with the capability for sampling large areas that are lightly loaded with microorganisms motivated the development of the vacuum probe. The intended use of the instrument is to sample clean surfaces in laminar flow clean rooms, but the device could be utilized for sampling surfaces in other clean environments. Such a device was designed, fabricated, and tested at Sandia Laboratories, Albuquerque, New Mexico. In these tests the vacuum probe removed a mean of 89% and assayed a mean of 67% of bacterial spores approximately 1 μ in length settled on smooth surfaces which were free of viscous films. Detailed machine and assembly drawings and instructions are included.

Project No. 0064010

* This work was conducted under Contract No. NASA R-09-019-040, Bioscience Division, Office of Space Science Application, NASA Headquarters, Washington, D. C.

ACKNOWLEDGMENT

We wish to express appreciation to
D. M. Garst, 1742 and K. F. Lindell, 1742,
for help in the preparation of this report.

TABLE OF CONTENTS

	Page
ACKNOWLEDGMENT	2
Introduction	5
Materials and Methods	7
Physical Description of Vacuum Probe	7
Microbiological Procedures	7
Results	11
Discussion	11
Machine and Assembly Drawings and Instructions	15
LIST OF REFERENCES	30

LIST OF FIGURES

Figure		Page
1	Assembled and Disassembled Vacuum Probes	6
2	Cross Section of Vacuum Probe Showing Airflow and a Detail View of the Teflon Tip	8
3	Effect of Airflow Rate Through Vacuum Probe on % Total Assay of Spores	13

AN IMPROVED MODEL OF THE VACUUM PROBE

Introduction

The recovery of microorganisms from surfaces has been studied by microbiologists since the early part of the century. During this period five basic methods have evolved for the microbiological examination of surfaces: the agar overlay method, the agar contact method, the swab-rinse method, the rinse method, and the agar-dip method.¹⁴ Each method has individual advantages and disadvantages, but all were designed for sampling relatively large populations of microorganisms on small to moderately sized surfaces.

The planetary quarantine requirement that space vehicles landing on planets designated as biological preserves be sterilized⁸ has imposed a requirement for the sampling of large surface areas with small amounts of microbial contamination.

The settling strip method¹² has been developed and used for estimating the viable contamination deposited on surfaces. With this method sterile stainless steel strips are placed in the same environment as the surface, and after a determined period of environmental exposure, the strips are assayed for microbial contamination. The criticisms of this method are that it is an indirect method and that it is inaccurate when the amount of microbial contamination is small.

The need for a microbiological surface sampling device with the capability for sampling large areas that are lightly loaded with microorganisms motivated the development of the vacuum probe sampler (Figure 1). The intended use of the instrument is to sample surfaces in laminar flow clean rooms.

For evaluation of the instrument a severe case was chosen, i. e., using settled-out aerosols of single Bacillus subtilis var. niger spores. In practice, however, few single spores or bacteria can be expected to settle out onto surfaces from the atmosphere. Nobel, et al¹¹ indicated that the majority of airborne microorganisms

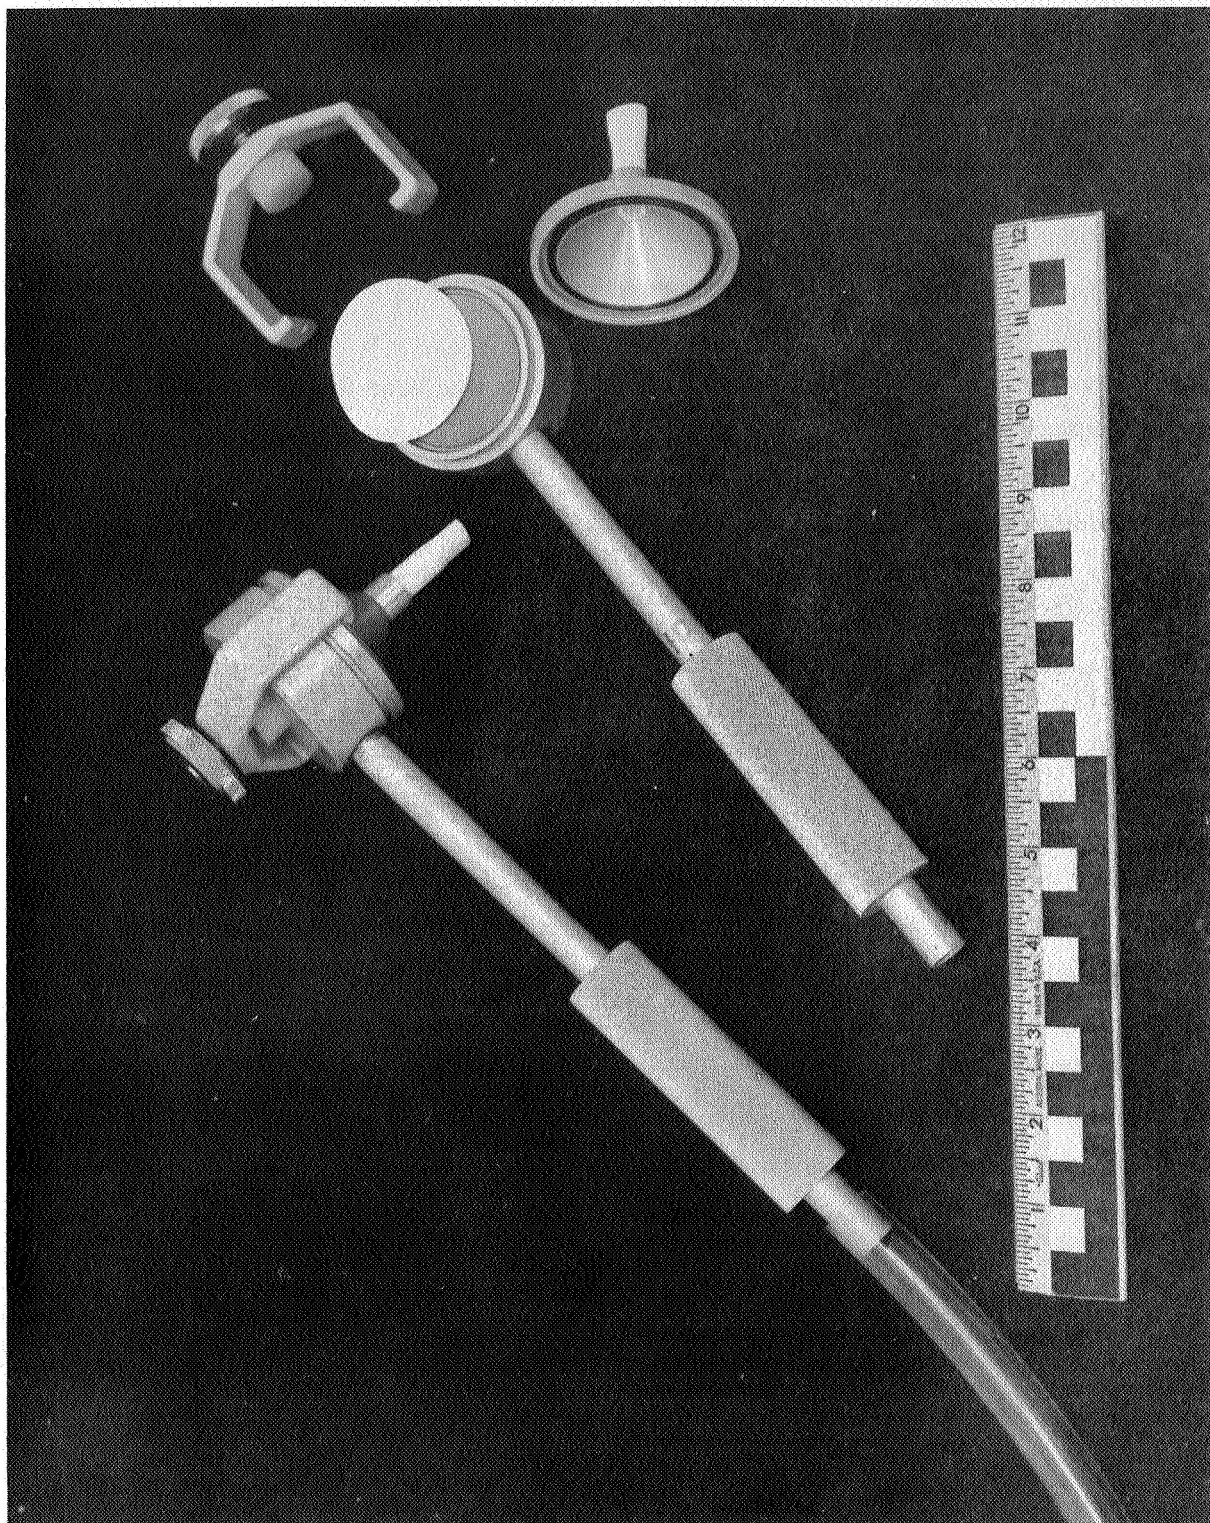


Figure 1. Assembled and Disassembled Vacuum Probes

in laboratory environments are carried on 4-20 μ diameter particles. Since the removal efficiency for particles remains consistently higher for larger particles^{3,4}, this evaluation was performed under the worst particle size conditions to be expected in practice.

Materials and Methods

Physical Description of Vacuum Probe

The vacuum probe (Figure 2) is an instrument that utilizes airflow through an orifice to remove particles from surfaces and a membrane filter to capture these particles. When the teflon tip (Figure 2 detail) contacts a surface, two orifices--one on the front side of the detail and one on the back--are formed. Since teflon has a low coefficient of friction with most materials, the tip is readily moved back-and-forth across surfaces for sampling. The cone is a machined and anodized aluminum-magnesium alloy casting which serves as a mechanical mount for the tip and holds an "O"-ring to seal the membrane filter to the filter backing screen. A two-inch-diameter membrane filter with a pore size of 0.45 μ or larger must be used or the filter limits the airflow excessively. A filter pore size should be selected, consistent with the particle size to be sampled. The filter backing screen is a circular piece of 100 mesh stainless steel screen clamped between an inner and outer ring. The filter backing screen is attached to the base with an autoclaveable epoxy adhesive (Shell Chemical Company, Epon 914). The base, which is also a machined and anodized aluminum-magnesium alloy casting, contains a plenum large enough to allow an even flow of air through the filter. The clamp holds the cone to the base, providing a rigid assembly and a good pressure seal. The anodized aluminum handle is sealed to the base using the same epoxy adhesive. The hollow handle serves to connect a vacuum system to the base during sampling.

Microbiological Procedures

All experimental procedures were carried out in a Class 100 laminar flow clean room⁶. This particular clean room^{2, 15} was well suited for such studies because of its size and airflow characteristics. Clean air flowing from one wall directly over the work surface to the floor allowed manipulations of contaminated test surfaces to be accomplished with minimal chance for additional contamination from personnel.

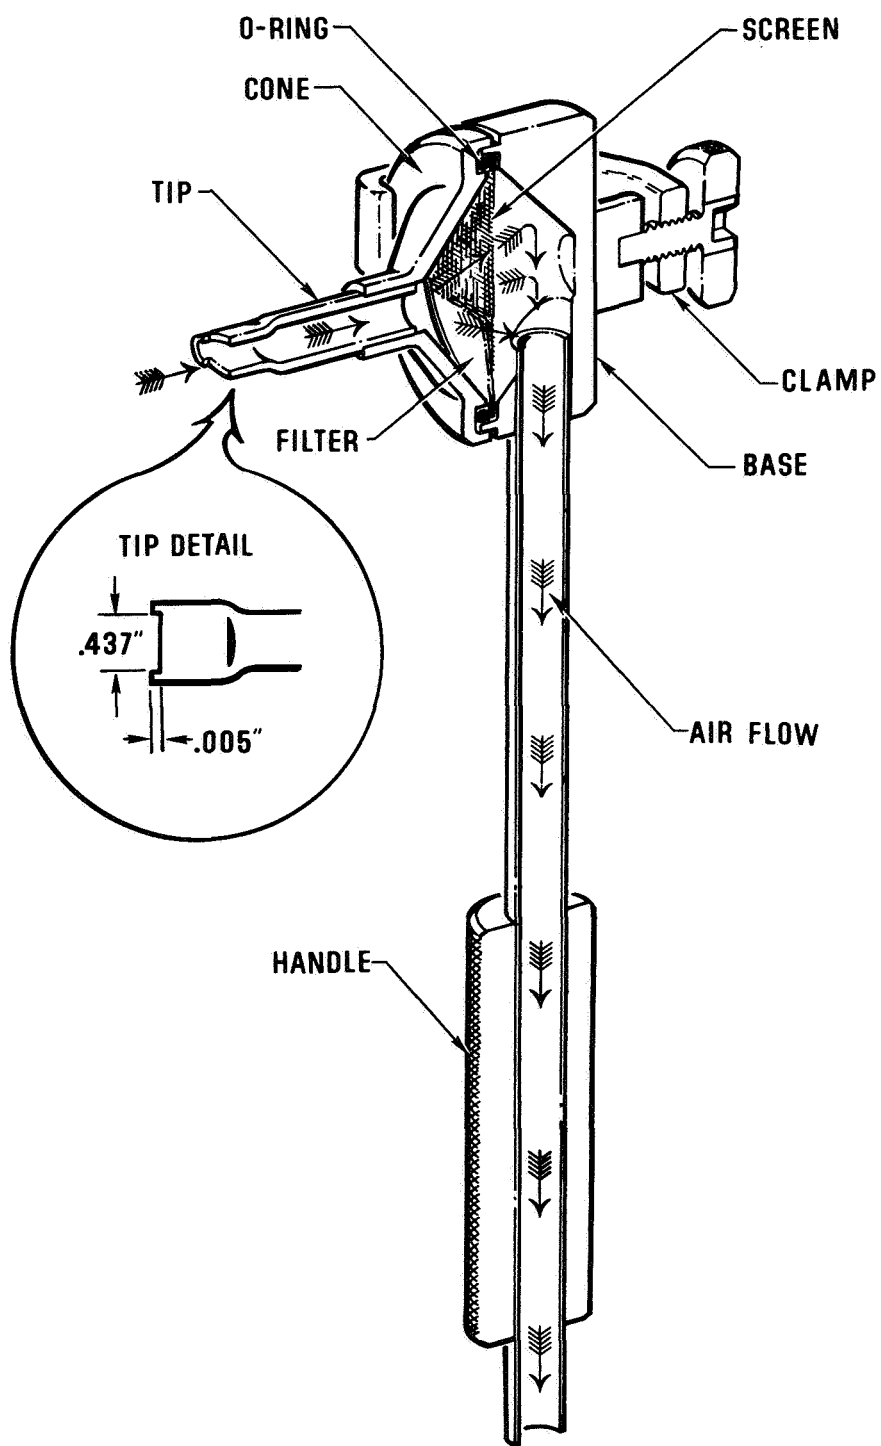


Figure 2. Cross Section of Vacuum Probe Showing Airflow and a Detail View of the Teflon Tip

The clean room was operated at all times, except during aerosolization and settling of particles. Just prior to aerosolization of bacterial spores, the clean room air circulation was turned off and spores were disseminated. After a settling period of 30 minutes, during which time the surfaces were contaminated with the test organisms, airflow was turned on and subsequent operations were performed in a clean air environment.

Bacillus subtilis var. niger spores suspended in 95% ethanol were disseminated with a DeVilbiss No. 40 nebulizer into a mixing fan which provided air circulation throughout the room. The fan was operated for one minute following aerosolization; then the spores were allowed to settle. The spore suspensions used were cleaned by insonation and differential centrifugation and were used in concentrations of 10^4 - 10^6 per ml. By microscopic observation the settled aerosol contained mostly single spores. By calculation, less than 1% of the spore-containing particles contained two spores and a negligible percentage contained more than two spores^{7,10}. For purposes of the experiment, the spores were free of ethanol on contact with the surface because the ethanol evaporated in a very short time compared to the settle-out time of the particles⁷.

The vacuum probe was sterilized and dried to remove any moisture. Sterile technique was followed in the installation of the 0.8μ pore size, two-inch diameter membrane filter. This pore size was suitable for filtering the spores. With the filter in place and the probe clamped together, the assembly was attached to a vacuum source. In normal use, a vacuum of 25 inches of mercury operating at a flow rate of approximately one cubic foot per minute was maintained. The probe tip was then placed in contact with and perpendicular to the surface to be sampled. A cross-hatched pattern was traced over the surface with the probe tip while maintaining the tip perpendicular to the sample surface. The crosshatched pattern was traced through twice, thus covering the sample surface two times in each direction. The teflon tip wears slowly and should be checked periodically. The rate of wear depends mainly on the force applied during sampling.

The probe was tested for efficiency of removal of spores from four different types of surfaces:

1. Glass — glass dishes 4" x 8-1/2" with a surface roughness height of 2.0μ inches.

2. Plastic — 20 mm x 150 mm disposable petri dishes with a surface roughness height of 5.5μ inches. A 4-inch square at the center of the plate was sampled.
3. Aluminum — 4" x 8-1/2" plates with a surface roughness height of 14.5μ inches.
4. Stainless Steel — 4" x 8-1/2" plates with a surface roughness height of 15.0μ inches.

Except for plastic, half of each surface was vacuumed with the other half serving as a control. Plastic dishes were vacuumed while adjacent dishes served as controls.

Surface contamination was assayed by overlaying the surface with sterile Trypticase Soy Agar (TSA;BBL), incubating at 32°C for 48-72 hr., and counting the colonies. To determine if the agar overlay procedure would move particles on the test surfaces, the sampled half of each surface was first crosshatched with molten TSA using a Cornwall syringe. After the TSA in the crosshatched portion had solidified, the entire surface was overlaid with more TSA. This crosshatching procedure prevented the possibility of washing viable particles from the sampled half to the control half of the test surface or vice versa. However, overlaying directly with agar had no noticeable effect on the spore distribution.

The metal surfaces were placed in sterile pans for vacuuming and for assay. After these pans were overlaid with TSA, they were left uncovered within the unoccupied, operating laminar flow clean room for approximately one hour to allow the surface of the TSA to dry. The pans were then covered with Saran Wrap and incubated at 32°C for 48-72 hr.

The cone and membrane filter were removed using sterile techniques. Spores collected on the membrane filter were assayed by overlaying the filter with TSA in a sterile petri dish, incubating at 32°C for 48-72 hr and counting the colonies developed.

According to N. L. Peterson's suggestion (U. S. P. H. S., N. C. D. C., Phoenix Field Station, Phoenix, Arizona; personal communication) the entire probe tip and cone were insonated. Insonation was performed for eight minutes in sterile 0.1% Tween 80, and the insonated fluid plated with TSA and incubated at 32°C for 48-72 hr. Later experiments, performed by vacuuming 5μ fluorescent particles and examining the interior of the vacuum probe with ultraviolet light, showed considerable particle

deposition on the inside surface of the cone and on the teflon tip. These experiments showed that the cone and tip would have to be insonated to raise total assay percentages.

In testing for percent assay as a function of percent of critical flow (Figure 3), an aerosol of 3×10^5 spores was settled on aluminum surfaces. The flow rate of air was varied with a flow meter.

Results

Table I shows sampling efficiencies on four different types of surfaces exposed to different levels of contamination. Particle removal efficiencies were consistently in excess of 80%, with a mean removal efficiency of 89%. Removal efficiencies appear to be independent of surface contamination densities studied. Total assay efficiencies were much more variable, but achieved a mean of 67% with a mean loss of 26% of those spores removed. Table I, as well as the fluorescent particle studies, shows that there was considerable deposition of particles on the inside surface of the cone and on the tip.

Figure 3 shows the decrease of total assay efficiency when the vacuum probe was operated with subcritical airflow rates at the tip.

Discussion

Since we were sampling from surfaces on which the loading density varied between test surface and control surface, assays of over 100% sometimes occurred. For the same reason we encountered removal efficiencies of greater than 100%; consequently, percentages of over 100% should not be interpreted as incorrect data, but are within the bounds of statistical variation.

Spores or other micron-sized particles on a smooth surface are difficult to disturb because the boundary layer of air near the surface is difficult to move and the small particles lie in the lower regions of this boundary. The force of adhesion between small particles and smooth surfaces is large compared to the normal aerodynamic forces encountered.³ The air entering the orifice when the tip touches a surface disturbs this boundary layer. The spores are dislodged and enter the moving airstream. The spores are then caught by a membrane filter.

TABLE I
Vacuum Probe Sampling Efficiencies
(*Bacillus subtilis* var. *niger* Spores)

Surface	Total Number of Spores Aerosolized	Unvacuumed		Vacuumed		Insonated Cone	% Removal ^a	Assay		
		Half	Half	Filter	Filter			% Total ^b	% Filter ^c	% Cone ^d
Aluminum	3 x 10 ⁵	89	5	51	8	94	66	57	9	
		129	5	104	32	96	105	81	24	
		149	13	76	27	91	69	51	18	
		<u>138</u>	<u>3</u>	<u>121</u>	<u>27</u>	<u>98</u>	<u>107</u>	<u>88</u>	<u>19</u>	
	Avg	126	6	88	24	95	89	70	19	
	3 x 10 ⁶	1550	76	430	368	95	52	28	24	
		886	88	428	414	90	95	48	47	
		1500	123	600	298	92	60	40	20	
		<u>1776</u>	<u>91</u>	<u>964</u>	<u>575</u>	<u>95</u>	<u>87</u>	<u>54</u>	<u>33</u>	
	Avg	1428	94	605	414	93	71	42	29	
Stain. Steel	3 x 10 ⁵	117	12	73	14	90	74	62	12	
		142	26	30	84	82	80	21	59	
		140	18	57	86	87	102	41	61	
		<u>150</u>	<u>16</u>	<u>86</u>	<u>34</u>	<u>89</u>	<u>80</u>	<u>57</u>	<u>23</u>	
	Avg	137	18	69	54	87	90	50	40	
Stain. Steel	3 x 10 ⁶	1400	154	393	207	89	43	28	15	
		1340	120	262	161	91	32	20	12	
		1600	145	516	414	91	58	32	26	
		<u>808</u>	<u>100</u>	<u>250</u>	<u>460</u>	<u>88</u>	<u>88</u>	<u>31</u>	<u>57</u>	
	Avg	1287	130	355	311	90	52	28	24	
Plastic	3 x 10 ⁴	17	5	7	9	71	94	41	53	
		40	4	5	7	90	30	12	18	
		34	5	2	9	85	32	6	26	
		<u>28</u>	<u>5</u>	<u>6</u>	<u>16</u>	<u>82</u>	<u>79</u>	<u>22</u>	<u>57</u>	
	Avg	30	5	5	10	84	50	17	33	
Glass	3 x 10 ⁶	828	130	245	138	84	46	30	16	
		1010	95	189	104	91	29	19	10	
		<u>800</u>	<u>155</u>	<u>231</u>	<u>161</u>	<u>81</u>	<u>49</u>	<u>29</u>	<u>20</u>	
	Avg	879	127	222	134	86	41	25	16	

a - % Removal = $\frac{\text{number on unvacuumed half of surface} - \text{number on vacuumed half of surface}}{\text{number on unvacuumed half of surface}} \times 100\%$

b - % Total = $\frac{\text{number on filter} + \text{number on cone}}{\text{number on unvacuumed half of surface}} \times 100\%$

c - % Filter = $\frac{\text{number on filter}}{\text{number on unvacuumed half of surface}} \times 100\%$

d - % Cone = $\frac{\text{number on cone and tip}}{\text{number on unvacuumed half of surface}} \times 100\%$

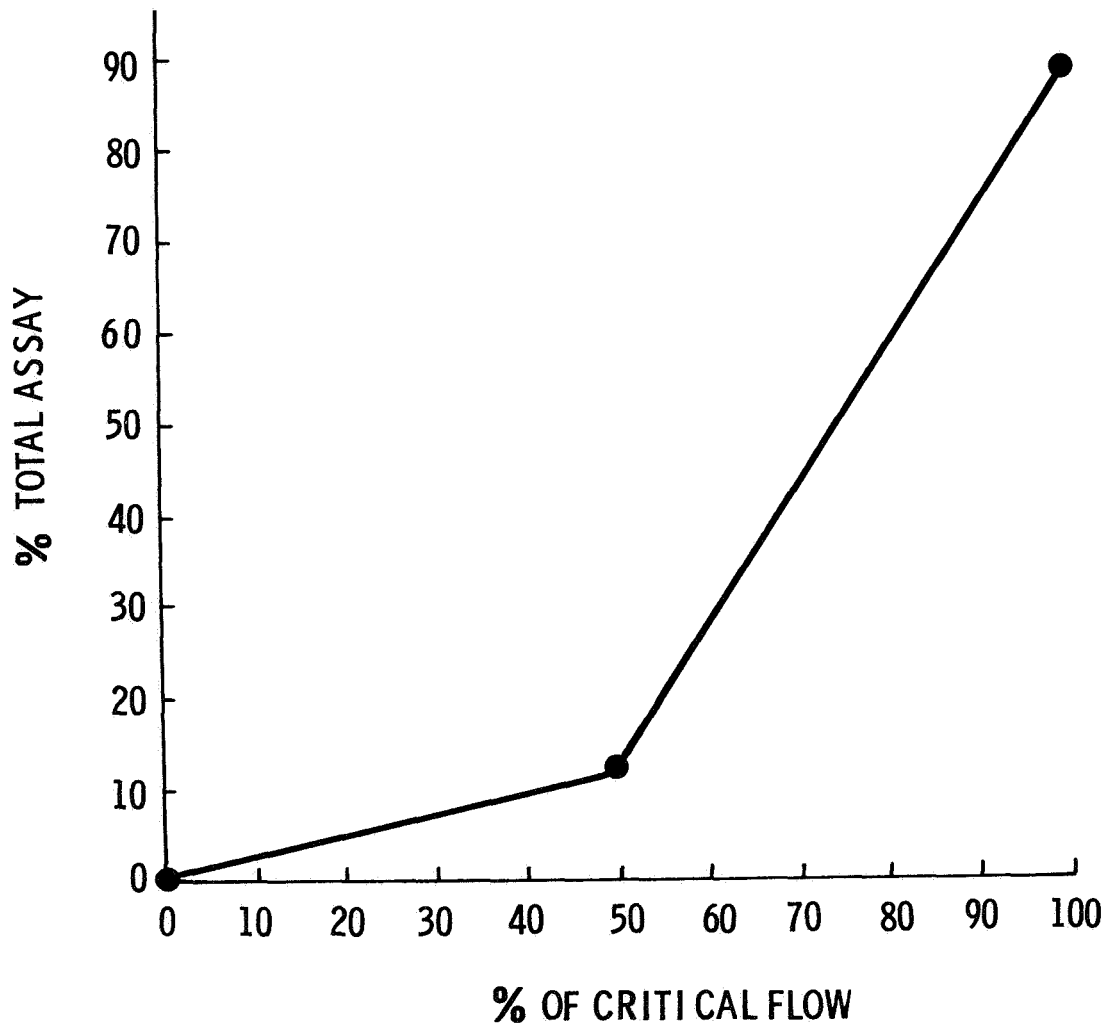


Figure 3. Effect of Airflow Rate Through Vacuum Probe on % Total Assay of Spores

A number of factors affect the removal and assay percentages in removing spores from different surfaces.

The most important criterion for high percentage removal and assay is that the two orifices in operation be at a critical flow rate. At critical flow, a shock wave is generated at the orifices. The air at the shock wave is very turbulent and tends to remove small particles effectively. The shock wave is generated if the ratio of the pressure inside the cone to atmospheric pressure is less than or equal to 0.528.¹³ All calibrations should be made with the filter in place. These values can be measured directly with a mercury manometer using a cone with a pressure fitting in the side. Figure 3 shows that critical flow must be reached to achieve high removal and assay percentages.

One anticipated problem was that particles were being overlaid with teflon from the tip during the sampling procedure. Studies with fluorescent powders $5\ \mu$ in diameter indicated that very few particles were overlaid with teflon. The fluorescent particles were placed on an aluminum surface and vacuumed under ultraviolet light. Traces of the powder showed where the teflon tip had passed, but the quantity was very small compared to the original loading. To further support these results, the experiment was repeated with a probe using a metal tip to eliminate teflon overlay. Removal percentages did not change significantly.

Another factor affecting removal percentages is particle size. Experimentation showed that the larger particles were easier to remove, so Bacillus subtilis var. niger spores approximately $1\ \mu$ in length were selected as the most difficult particle to remove.^{3, 4}

At the present time we have done very little work using spores overlaid with thin films such as oily handprints. Limited experimentation suggested that these particles were more difficult to remove.^{3, 4}

Electrostatic charges affected some experiments, especially those on glass and plastic surfaces, but the effects were not measured quantitatively. In some instances, very strong fields--strong enough to push the membrane filter from the bottom to the top of the petri dish in which it was laying before overlay--were generated on the filters and petri dishes. In general, aerosols generated by blasting particles with air have a fairly high density charge distribution;⁹ therefore, part of the variation in assay percentages is possibly a result of interacting electrostatic forces along with aerodynamic forces. The electrostatic forces may explain the lower assay percentages on plastic.

Three other effects of interest are relative humidity, surface roughness, and the natural adhesiveness between particular pairs of materials. Although all of this work was done at 45% relative humidity, Corn³ reported that particle adhesiveness generally increases as humidity increases. The effect of surface roughness was poorly defined in our experiments; however, Corn³ indicated that adhesion decreases as surface roughness increases. The surface roughness heights¹ of the surfaces used are given. Adhesive forces vary considerably for different pairs of materials.³

We have modified the vacuum probe to provide a clean air sheath so that the device can be used to sample surfaces in environments other than those provided by

laminar flow rooms. We are also developing a method to impinge the particles directly onto agar nutrient rather than onto a filter which is then plated in agar nutrient.


Machine and Assembly Drawings and Instructions

The teflon tip was machined from commercially available teflon tubing with nominal dimensions of 0.400 inch outside diameter by 0.214 inch inside diameter. After machining the threads and tubing to length 0.400 inch of the teflon was placed in a vise and clamped flat. The tip was then placed in a cone, used as a machining jig. The slot in the tip was machined using a 7/16- inch bit in an end mill. A first pass with the tool was made to cut the tip flat, and a second pass was made to cut the slot.


The inner and outer screen ring and the screen were assembled with a press.

An epoxy glue (Shell Chemical Company, Epon 914) was used to attach both the screen assembly and the handle to the base. The epoxy was cured at 350°F for two hours.


Item and assembly drawings follow.

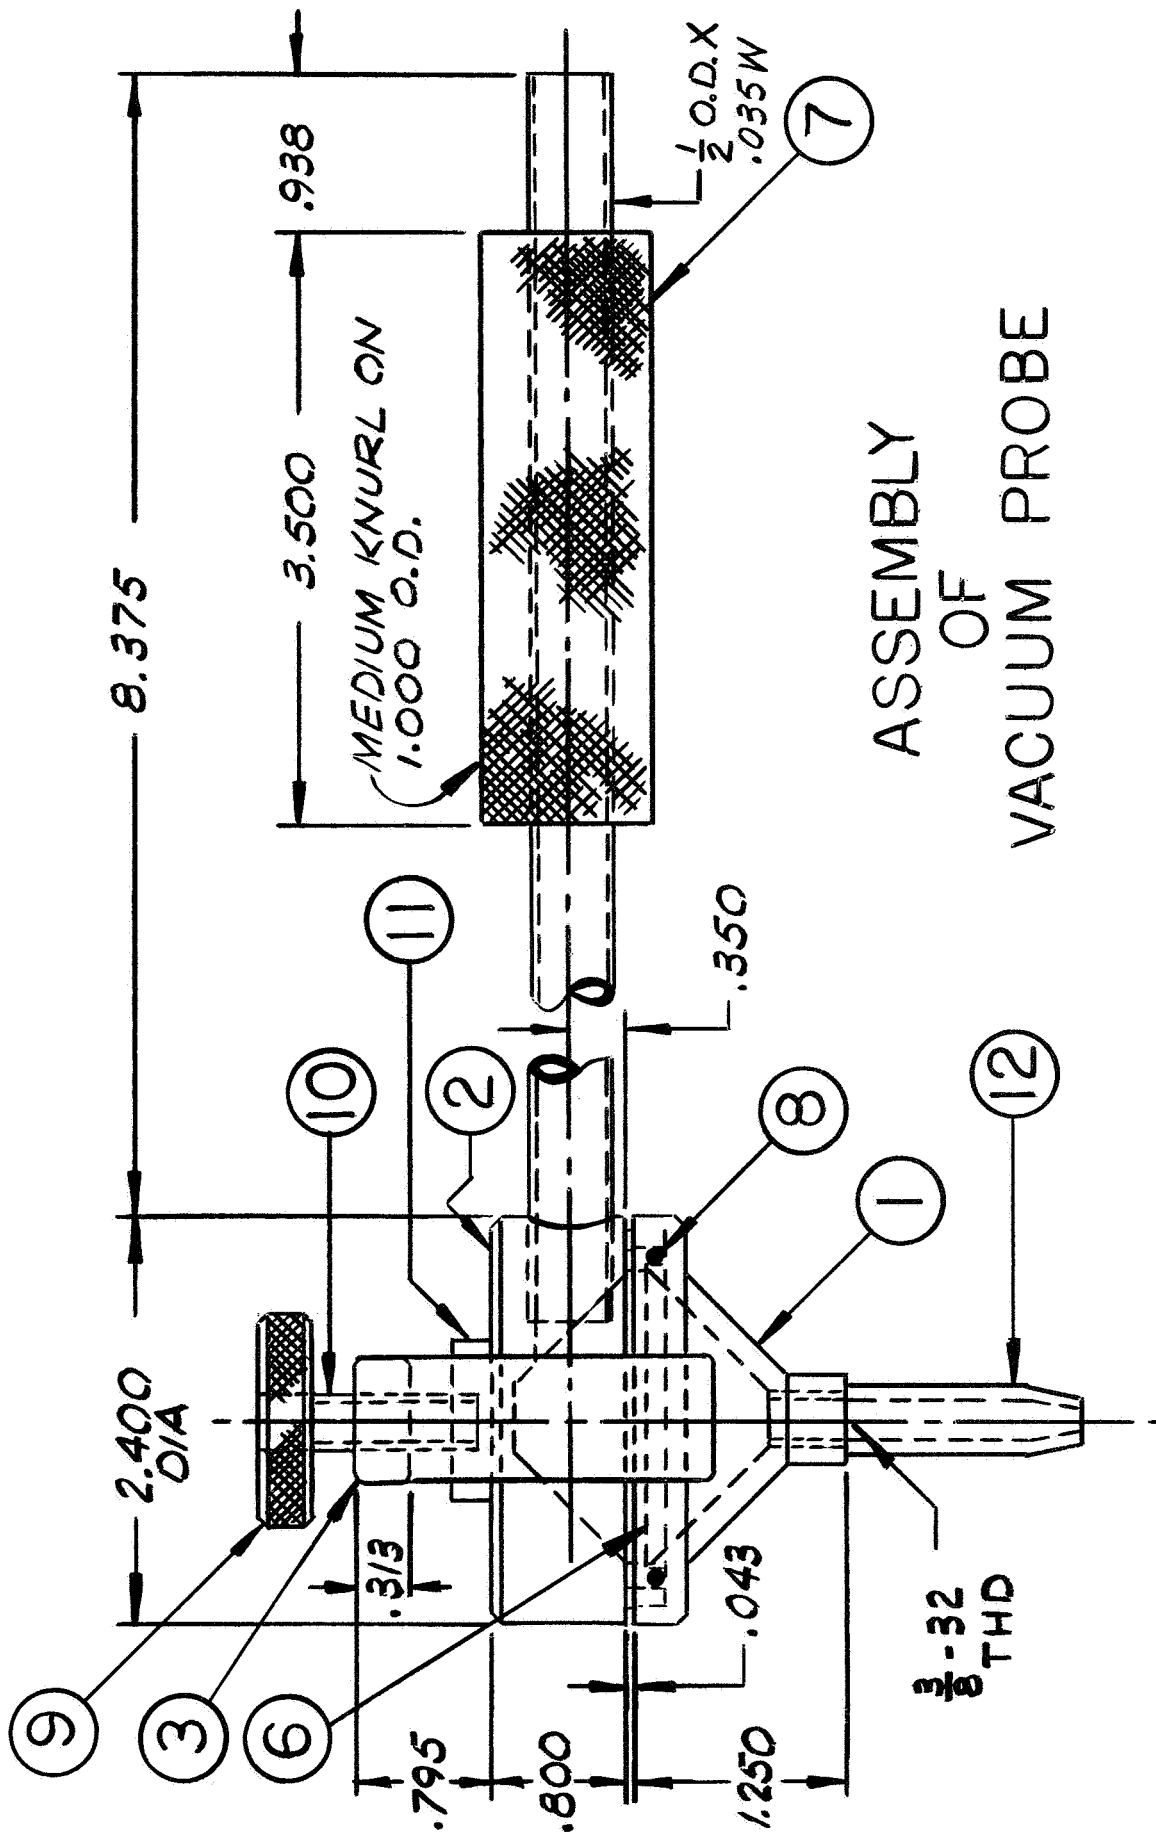

ASSEMBLY
OF
VACUUM PROBE

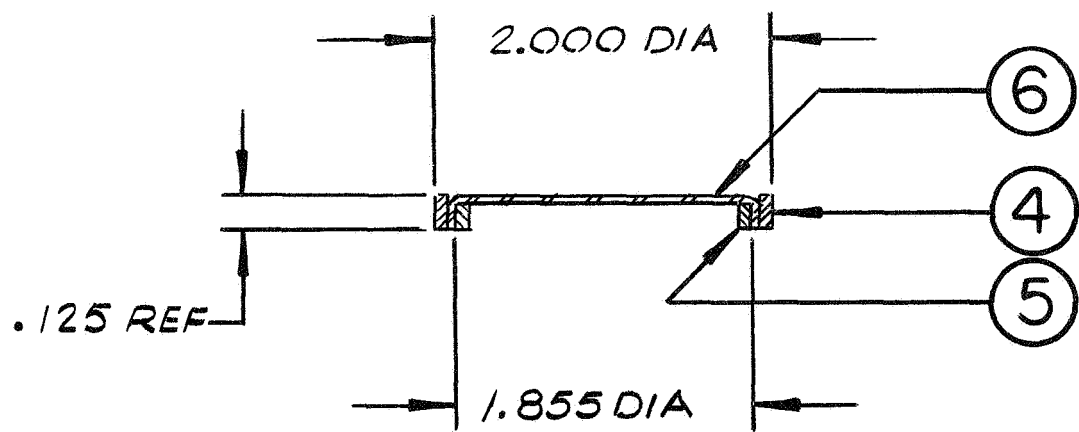


SCREEN ASSEMBLY

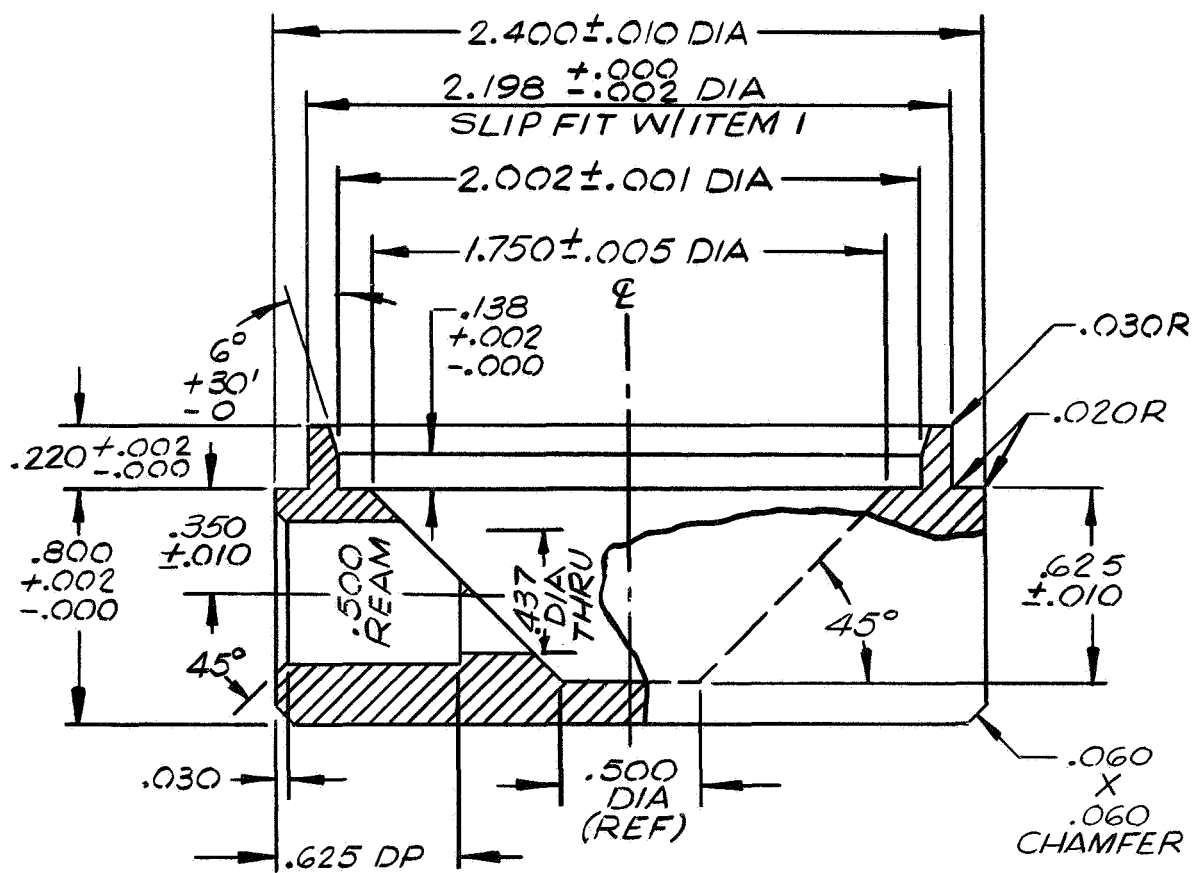


MATERIAL: ALUMINUM

ITEM 2

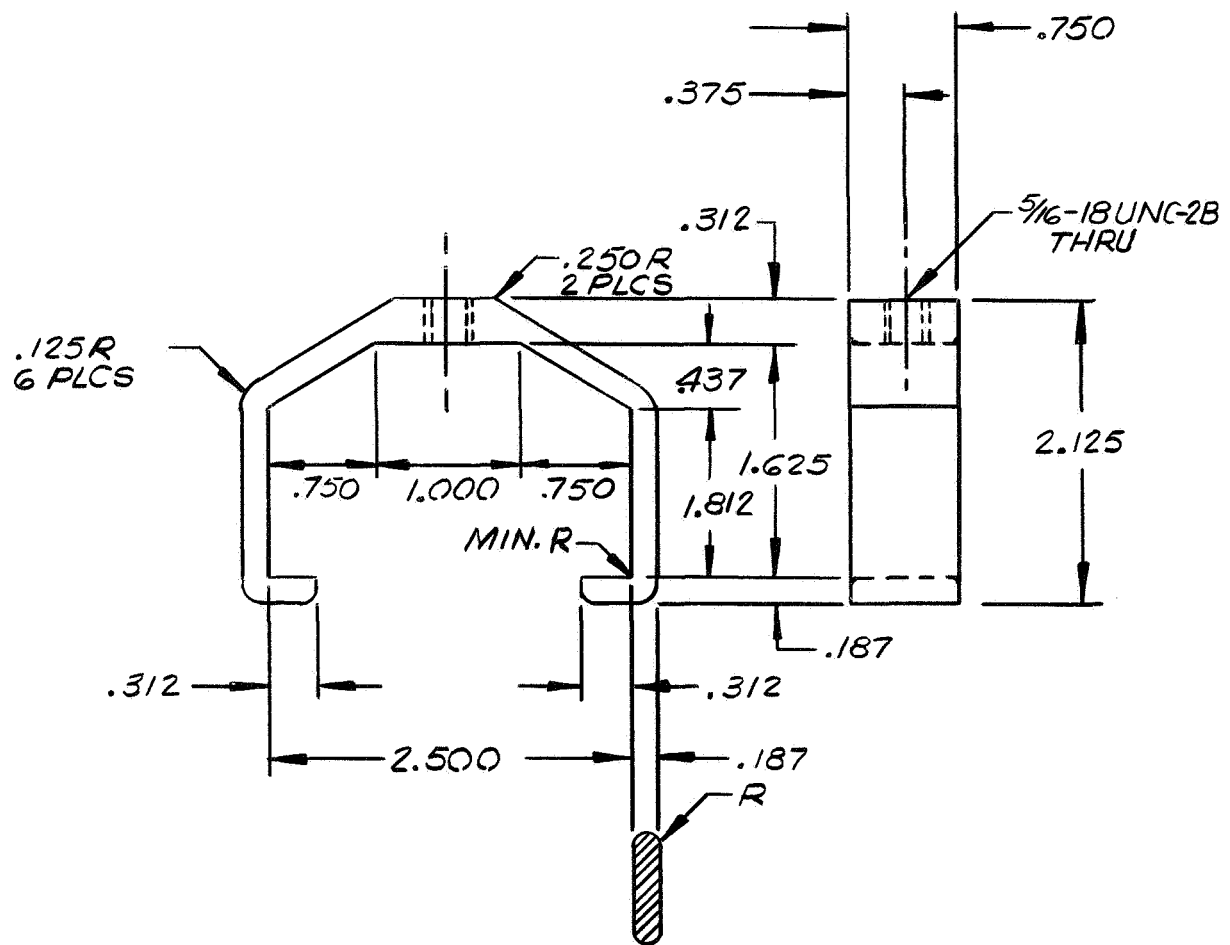


MATERIAL: ALMAG CASTING

ITEM 3

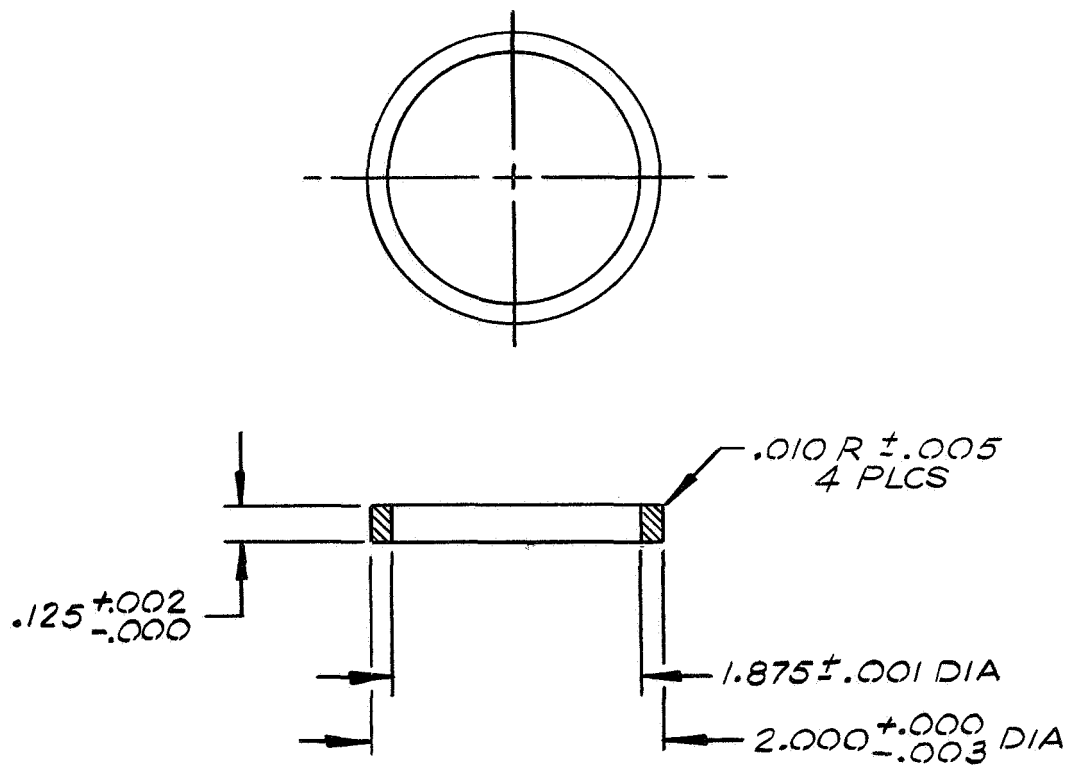


MATERIAL: STAINLESS STEEL, 303

ITEM 4

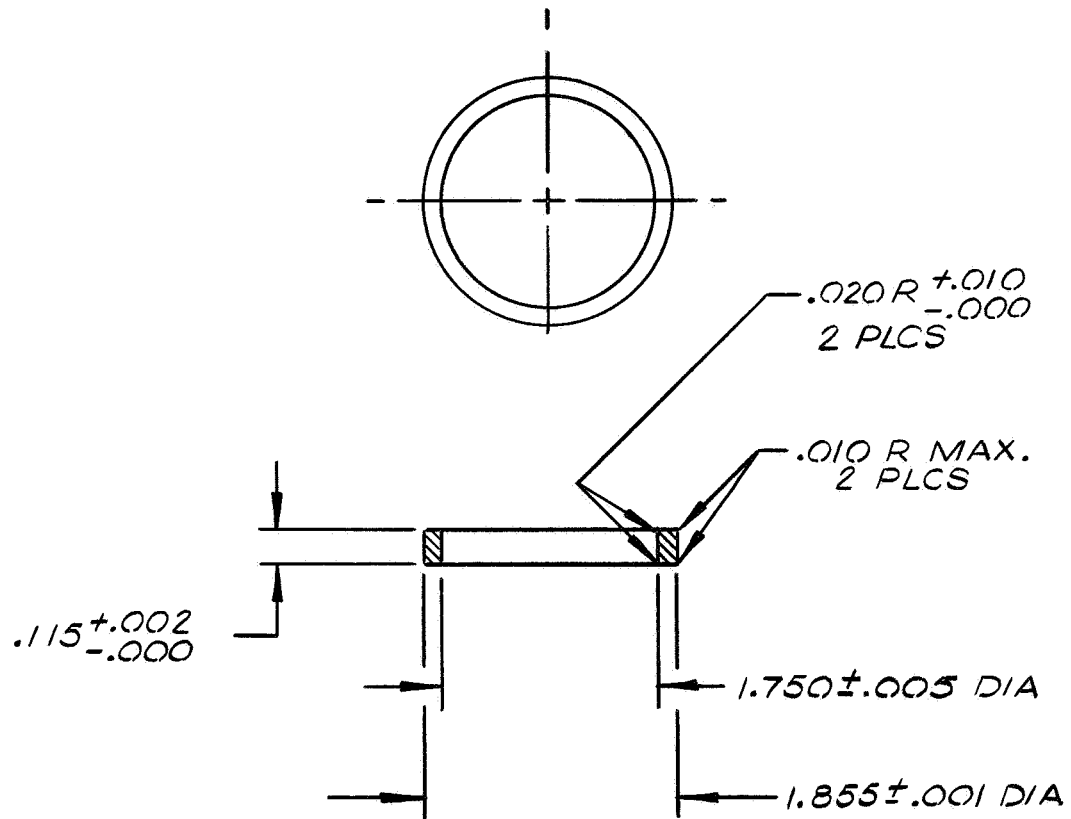


MATERIAL: STAINLESS STEEL, 303

ITEM 5

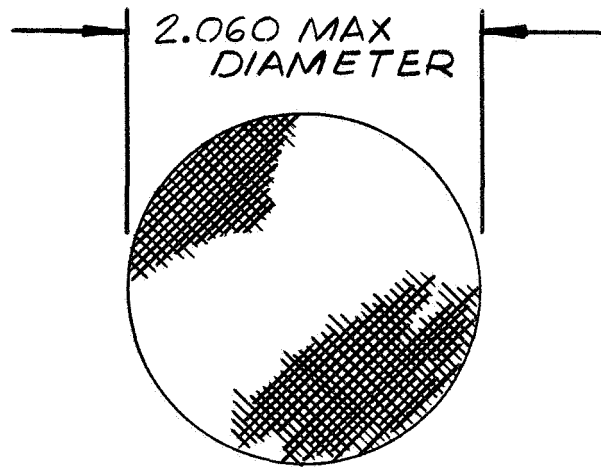


*MATERIAL: 100 MESH STAINLESS
STEEL SCREEN*

ITEM 6

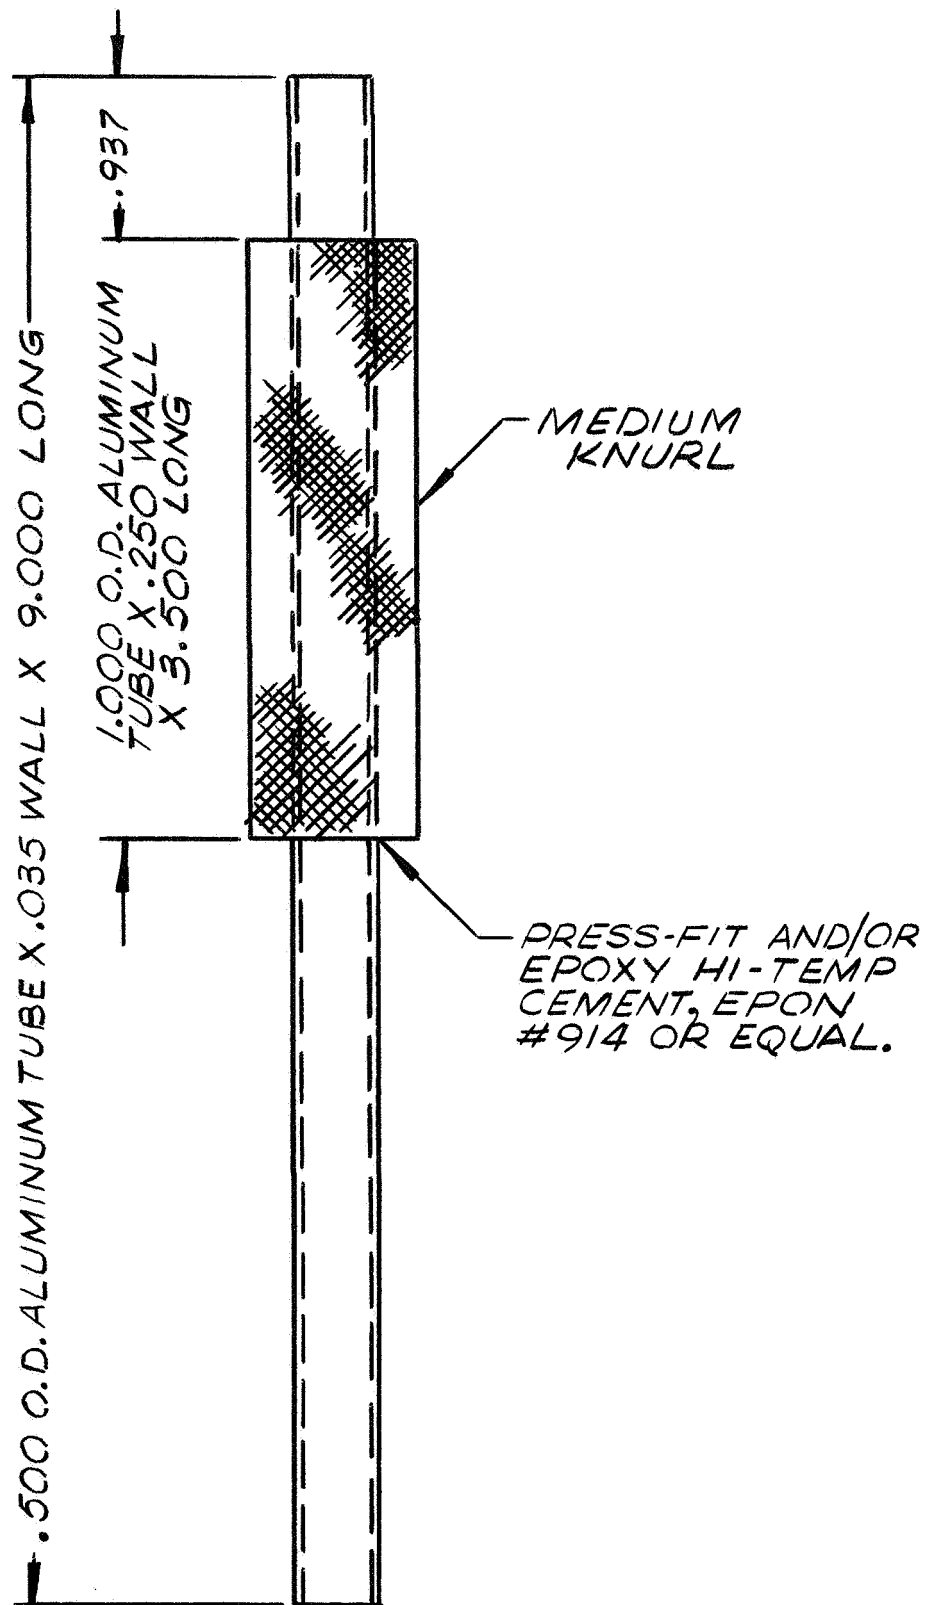


ITEM 7

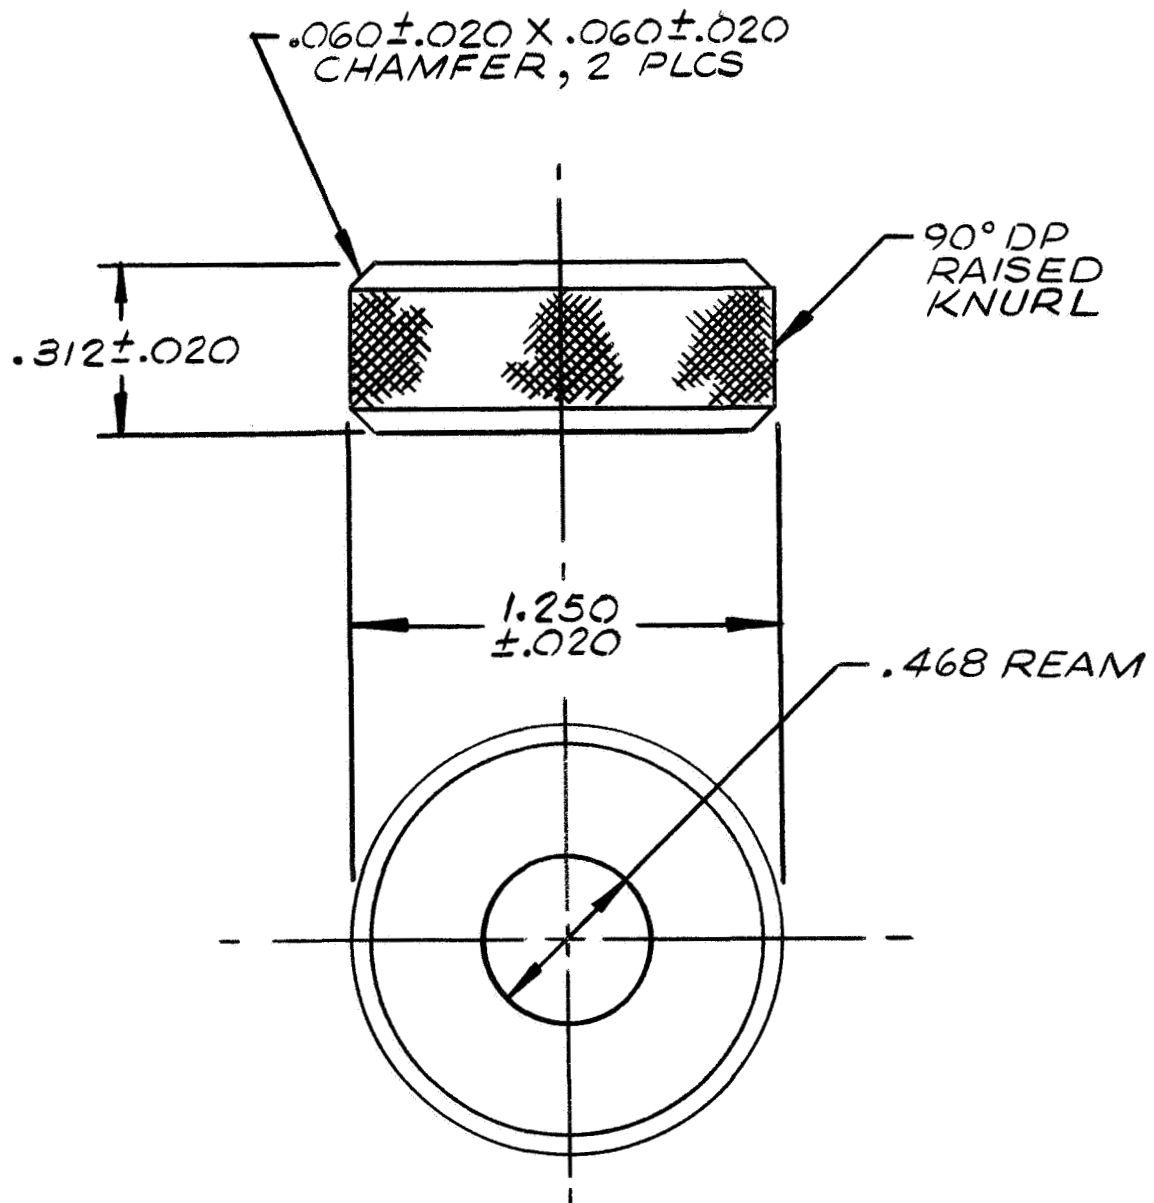


MATERIAL: BRASS, 1/2 HARD

ITEM 9

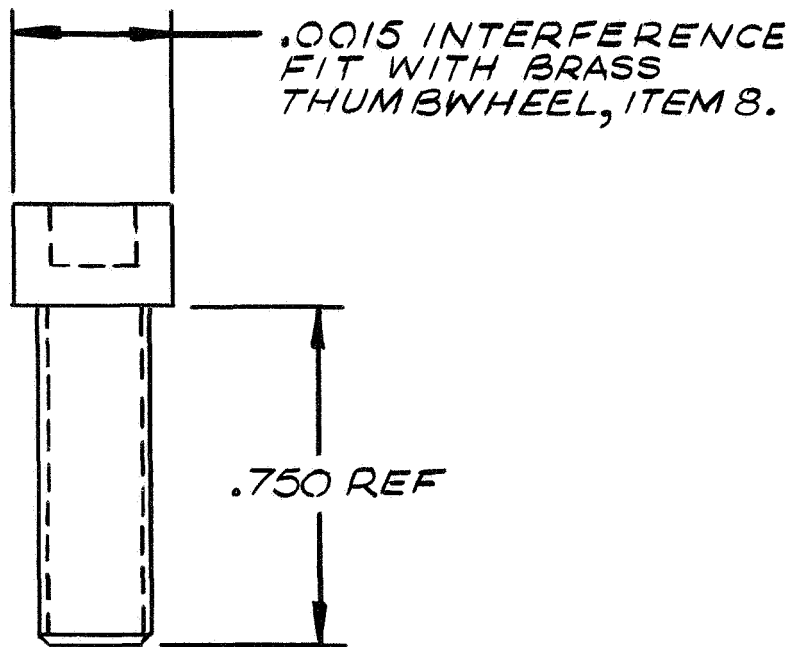



MATERIAL: SOCKET HD CAP SCREW, 5/16-18 UNC X 3/4 LG.

ITEM 10

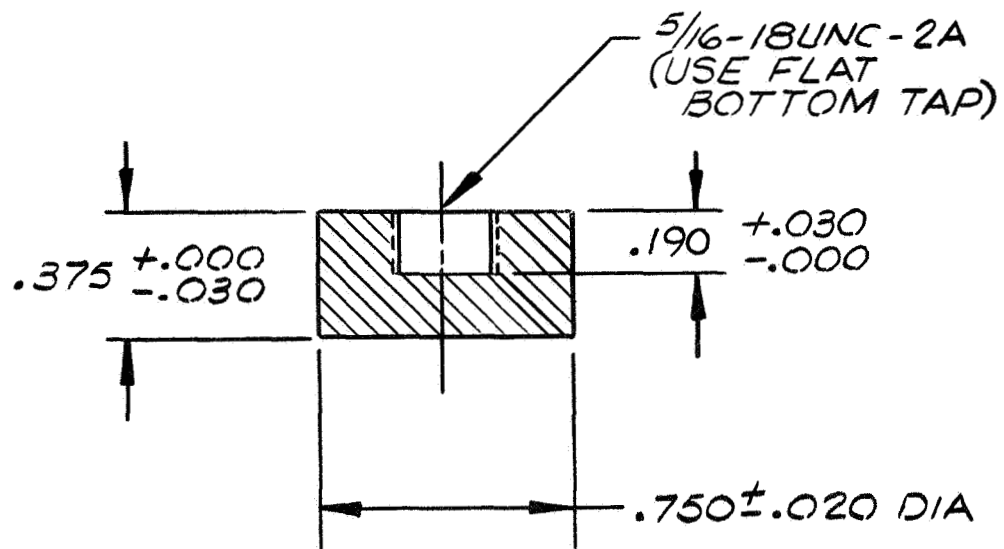

MATERIAL: NYLON ROD

ITEM 11

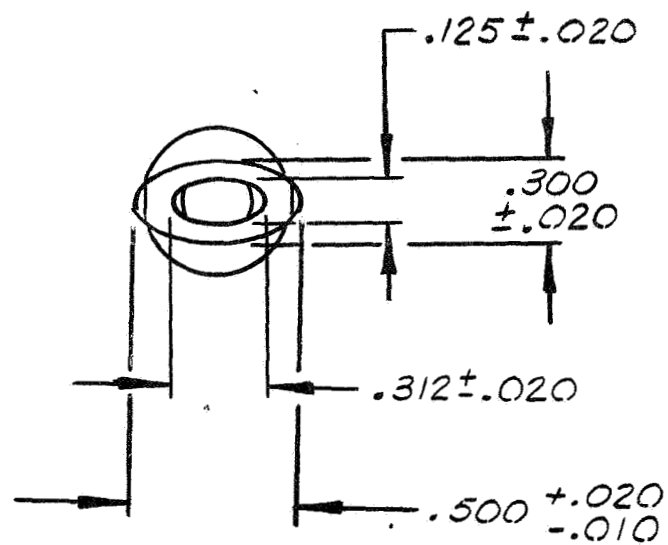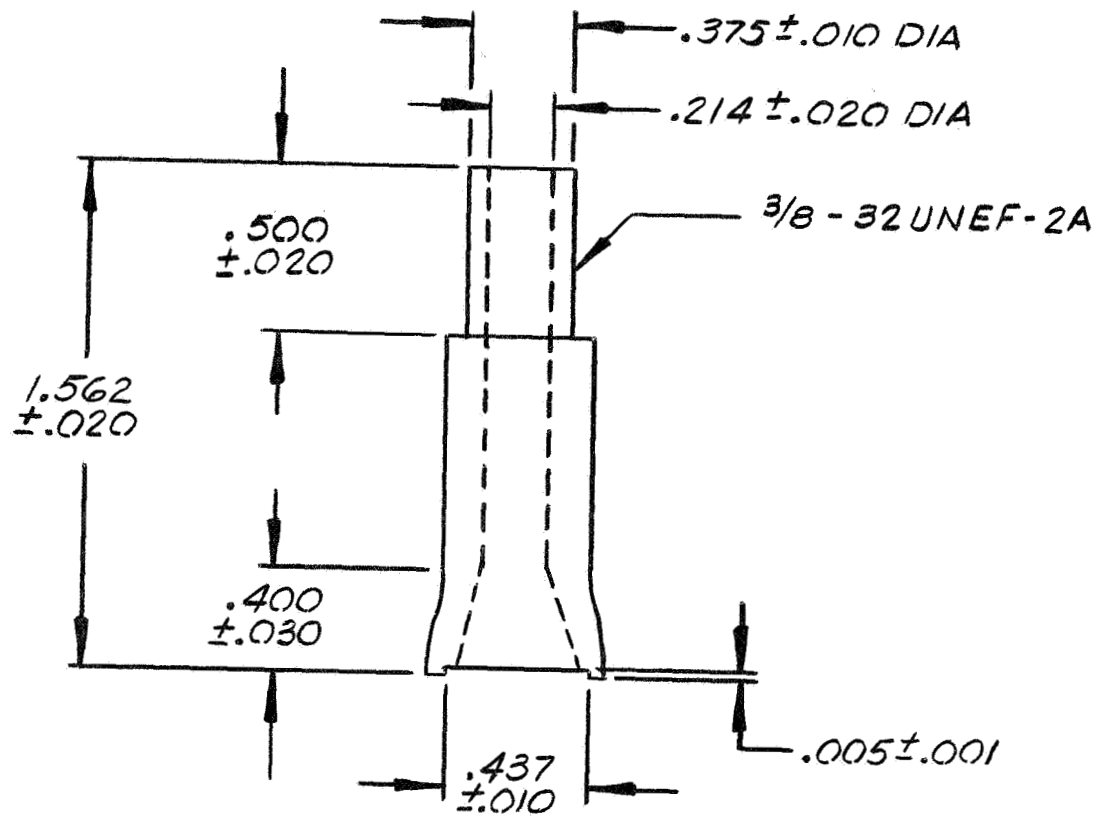

ITEM 12

LIST OF REFERENCES

1. American Standard No. ASA B46.1-1962. 1962. Surface Texture. The American Society of Mechanical Engineers, United Engineering Center, New York 17, New York, 27 p.
2. Beakley, J. W., W. J. Whitfield, and J. C. Mashburn. 1966. Evaluation of the efficiency of a Class 100 laminar-flow clean room for viable contamination cleanup. Sandia Corp. Res. Rep. No. SC-RR-66-385.
3. Corn, M. 1967. Adhesion of particles, p. 359-392. In C. N. Davies, editor Aerosol Science. Academic Press, New York.
4. Dugan, V. L., W. J. Whitfield, J. J. McDade, J. W. Beakley, and F. W. Oswalt. 1967. A new approach to the microbiological sampling of surfaces: The vacuum probe sampler. Sandia Corp. Res. Rep. No. SC-RR-67-114.
5. Dugan, V. L. 1967. Principles of operation of the vacuum probe microbiological sampler. Sandia Corp. Res. Rep. No. SC-RR-67-688.
6. Federal Standard No. 209a. 1966. General Services Administration, Business Service Center, Washington, D. C. 21 p.
7. Green, H. L. and W. R. Lane. 1964. Particulate clouds: Dusts, smokes, and mists. Van Nostrand, New Jersey. 471 p.
8. Hall, L. B. 1966. NASA requirements for the sterilization of spacecraft, p. 25-39. In Spacecraft sterilization technology. NASA SP-108. Office of Technology Utilization, National Aeronautics and Space Administration, Washington, D. C.
9. Kunkel, W. B. 1950. The static electrification of dust particles on dispersion into a cloud. J. Appl. Phys. 21: 820-832.
10. Mercer, T. T., M. I. Tillery, and H. Y. Chow. 1968. Operating characteristics of some compressed-air nebulizers. Amer. Ind. Hyg. Assn. J. 29: 66-78.
11. Noble, W. C., O. M. Lidwell, and D. Kingston. 1963. The size distribution of airborne particles carrying microorganisms. J. Hyg., Camb. 61: 385-391.

12. Portner, D. M., Hoffman, R. K., and Phillips, C. R. 1965. Microbial control in assembly areas needed for spacecraft sterilization. *Air Eng.* 7(10): 46-49.
13. Shames, I. H. 1962. One-dimensional compressible flow, p. 392-449. In I. H. Shames, *Mechanics of fluids*. McGraw, New York.
14. Vesley, D. 1966. Survey of microbiological techniques for recovery from surfaces, p. 147-153. In *Spacecraft Sterilization Technology*. NASA SP-108. Office of Technology Utilization, National Aeronautics and Space Administration, Washington, D.C.
15. Whitfield, W. J. 1962. A new approach to clean room design. Sandia Corp. Res. Rep. No. SC-4673(RR).

DISTRIBUTION:

NASA, Code SC
Grants and Contracts
400 Maryland Avenue, S.W.
Washington, D. C. 20546 (25)

L. B. Hall, NASA
Code SB
400 Maryland Avenue, S.W.
Washington, D. C. 20546 (25)

E. D. Smyth
Acting Chief, Special Projects Branch
Sandia Area Office
U.S. Atomic Energy Commission
Albuquerque, New Mexico 87115

S. A. Upson
Director, Non Weapons Activity Division
Office of Plans and Budgets
U.S. Atomic Energy Commission
Albuquerque, New Mexico 87115

Harold Walker
Director of Research Services
Graduate College
University of New Mexico
Albuquerque, New Mexico

University of California, LRL
P.O. Box 808
Livermore, California 94551
Attn: Technical Information Division
For: Report Librarian

Los Alamos Scientific Laboratory
P.O. Box 1663
Los Alamos, New Mexico
Attn: Report Librarian

Richard G. Bond
School of Public Health
College of Medical Science
University of Minnesota
Minneapolis, Minnesota 55455

John H. Brewer
Biological Safety and Control
Becton, Dickinson and Company
P.O. Box 6711
Baltimore, Maryland 21204

Frank B. Engley, Jr.
Chairman, Department of Microbiology
School of Medicine
University of Missouri
Columbia, Missouri

Gilbert V. Levin
Hazleton Laboratories, Inc.
Box 30
Falls Church, Virginia

Irving J. Pflug
Professor of Environmental Health
University of Minnesota
College of Medical Sciences
Minneapolis, Minnesota 59455

Gerald Silverman
Department of Nutrition and Food Science
Massachusetts Institute of Technology
Cambridge, Massachusetts 02139

John A. Ulrich
Department of Microbiology
May Clinic
Rochester, Minnesota 55902

Samuel Schalkowsky
Exotech Incorporated
525 School Street, S. W.
Washington, D. C. 20024

Charles Craven
Jet Propulsion Laboratory
4800 Oak Grove Dr.
Pasadena, California 91103

Mark A. Chatigny
Research Engineer
Naval Biological Laboratory
Naval Supply Center
University of California, Berkeley
Oakland, California 94625

Richard G. Cornell
Associate Professor of Statistics
Department of Statistics
Florida State University
Tallahassee, Florida

Martin S. Favero
Department of Health, Ed. and Welfare
CDC-Phoenix Field Station
4402 North 7th Street
Phoenix, Arizona 85014

F. N. LeDoux
Head, Structural and Mechanical
Applications Section
Goddard Space Flight Center
Greenbelt, Maryland

DISTRIBUTION: (Cont.)

Q. Ussery
CodeNC-3, Quality Assurance Branch
Manned Spacecraft Center, NASA
Houston, Texas

F. J. Beyerle
George C. Marshall Space Flight Center
Manufacturing Engineering Laboratory
M/F Building 4471
Huntsville, Alabama 35812

J. Gayle
Code SOP
Kennedy Space Center, NASA
Cape Kennedy, Florida

E. Rich
Code 624
GSFC Sterilization Laboratory
Goddard Space Flight Center
Greenbelt, Maryland 20771

N. H. MacLeod
Space Biology Branch
Code 624, Bldg. 21, Rm. 161
Goddard Space Flight Center
Greenbelt, Maryland 20771

Robert Angelotti
Deputy Chief, Milk and Food Research
Robert A. Taft Sanitary Engineering
Center
Cincinnati, Ohio

Erwin Fried
Rm. M-2101
General Electric Company
P. O. Box 8555
Philadelphia, Pennsylvania 19101

Martin G. Koesterer, Microbiologist
Bioscience Operation
General Electric
P. O. Box 8555
Philadelphia, Pennsylvania 19101

Carl Bruch
Chief, Bacteriology Branch
Division of Microbiology
Food and Drug Administration
3rd and C., SW, Room 3876
Washington, D. C. 20204

John W. Beakley
Department of Biology
University of New Mexico
Albuquerque, New Mexico

Loren D. Potter, Chairman
Department of Biology
University of New Mexico
Albuquerque, New Mexico

Loris W. Hughes
Department of Biology
New Mexico State University
University Park, New Mexico

Joe Stern
Jet Propulsion Laboratory
4800 Oak Grove Dr.
Pasadena, California 91103

Edwin J. Sherry
Jet Propulsion Laboratory
4800 Oak Grove Dr.
Pasadena, California 91103

J. J. McDade
Biohazards Group
Pitman-Moore Company
Dow Chemical Company
P. O. Box 1656
Indianapolis, Indiana 46206

William K. McKim
Aerospace Corporation
Building A2, Room 2019
2350 East E1 Segundo Blvd.
El Segundo, California

James A. Green
Life Sciences Systems (BB14)
North American Rockwell Corp.
12214 Lakewood Blvd.
Downey, California

Fred L. Whipple
Smithsonian Astrophysical Observatory
Cambridge, Massachusetts 02138

Arthur H. Neill, NASA
Code SB
400 Maryland Avenue, S.W.
Washington, D. C. 20546

Adelbert L. Roark
West Virginia University
Mathematics Department
Morgantown, West Virginia 26506 (6)

Rudy Puleo
Public Health Service
Spacecraft Bioassay Laboratory
Drawer Y
Cape Canaveral, Florida 32900

DISTRIBUTION: (Cont.)

Virgil Dugan
Department of Electrical Engineering
Mississippi State University
State College, Mississippi 39762

Carl Sagan
Department of Astronomy
Cornell University
Ithaca, New York 14850

USAEC

Division of Technical Information
P.O. Box 62
Oak Ridge, Tennessee 37830
Attn: Reference Branch
P. E. Postell

J. A. Hornbeck, 1
W. J. Howard, 1000
W. A. Gardner, 1500
H. E. Lenander, 1600
T. M. Burford, 1700
J. W. Weihe, 1710
D. P. Peterson, 1711
M. J. Norris, 1720
J. M. Worrell, Jr., 1721
H. D. Sivinski, 1740 (20)
D. R. Cotter, 1800
B. H. Van Domelen, 1830
R. T. Dillon, 1830
R. W. Henderson, 2000
L. A. Hopkins, 2300
J. W. Jones, 2350
L. J. Paddison, 2400
R. S. Claassen, 2600
J. R. Sublett, 2640
R. B. Powell, 3000
C. W. Campbell, 4000
S. J. Buchsbaum, 5000
L. C. Hebel, 5200
C. F. Bild, 5400
D. W. Ballard, 5414
R. A. Bice, 7000
L. E. Lamkin, 7300
L. J. Heilman, 7400
C. R. Barncord, 7600
J. R. Meikle, 7640
G. A. Fowler, 9000
J. H. Scott, 9200
A. Y. Pope, 9300
J. W. McKiernan, 9521
W. F. Carstens, 3410
L. C. Baldwin, 3412
W. J. Wagoner, 3413
For: DTIE (3)
M. S. Goldstein (1)
B. R. Allen, 3421
B. F. Hefley, 8232
C. H. Sproul, 3428-2 (10)