

N O T I C E

THIS DOCUMENT HAS BEEN REPRODUCED FROM
MICROFICHE. ALTHOUGH IT IS RECOGNIZED THAT
CERTAIN PORTIONS ARE ILLEGIBLE, IT IS BEING RELEASED
IN THE INTEREST OF MAKING AVAILABLE AS MUCH
INFORMATION AS POSSIBLE


NO2 Heterodyne Frequency Measurements with a
Tunable Diode Laser, a CO Laser
Transfer Oscillator, and CO2 Laser Standards

(U.S.) National Bureau of Standards (NML)
Boulder, CO

Prepared for

National Aeronautics and Space Administration
Washington, DC

Apr 87

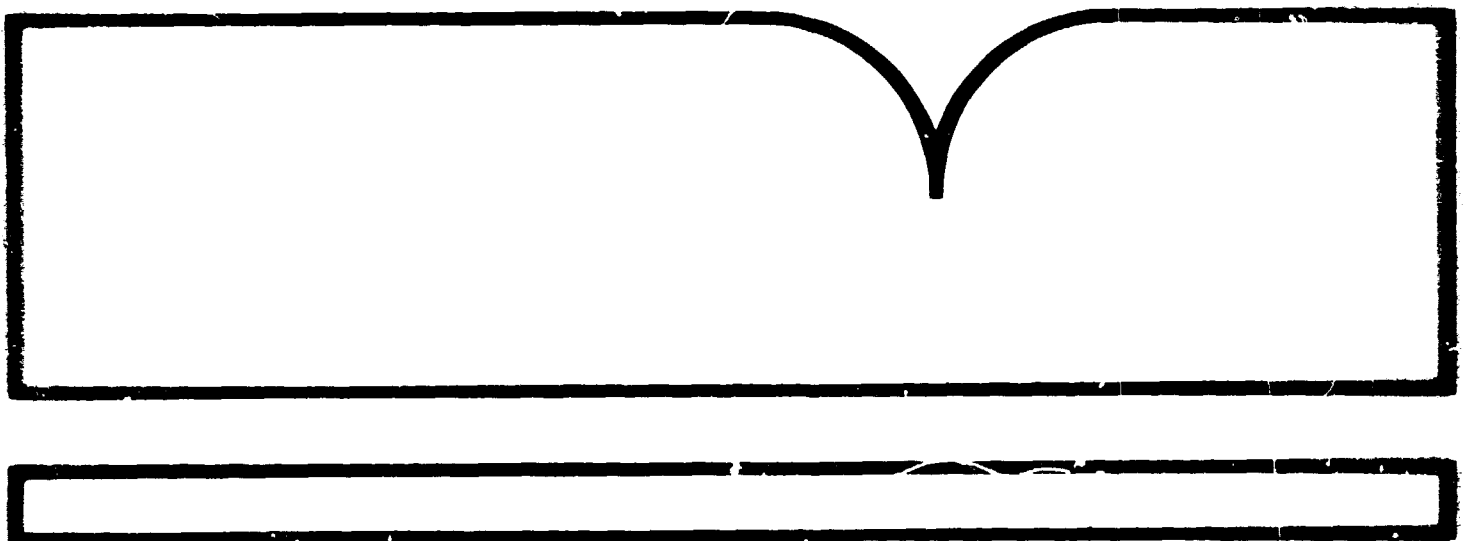



NBS TECHNICAL NOTE 1308

U.S. DEPARTMENT OF COMMERCE / National Bureau of Standards

NO₂ Heterodyne Frequency Measurements With a Tunable Diode Laser, a CO Laser Transfer Oscillator, and CO₂ Laser Standards

L.R. Zink
M. Vanek
J.S. Wells

The National Bureau of Standards¹ was established by an act of Congress on March 3, 1901. The Bureau's overall goal is to strengthen and advance the nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research to assure international competitiveness and leadership of U.S. industry, science and technology. NBS work involves development and transfer of measurements, standards and related science and technology, in support of continually improving U.S. productivity, product quality and reliability, innovation and underlying science and engineering. The Bureau's technical work is performed by the National Measurement Laboratory, the National Engineering Laboratory, the Institute for Computer Sciences and Technology, and the Institute for Materials Science and Engineering.

The National Measurement Laboratory

Provides the national system of physical and chemical measurement; coordinates the system with measurement systems of other nations and furnishes essential services leading to accurate and uniform physical and chemical measurement throughout the Nation's scientific community, industry, and commerce; provides advisory and research services to other Government agencies; conducts physical and chemical research; develops, produces, and distributes Standard Reference Materials; provides calibration services; and manages the National Standard Reference Data System. The Laboratory consists of the following centers:

- Basic Standards²
- Radiation Research
- Chemical Physics
- Analytical Chemistry

The National Engineering Laboratory

Provides technology and technical services to the public and private sectors to address national needs and to solve national problems; conducts research in engineering and applied science in support of these efforts; builds and maintains competence in the necessary disciplines required to carry out this research and technical service; develops engineering data and measurement capabilities; provides engineering measurement traceability services; develops test methods and proposes engineering standards and code changes; develops and proposes new engineering practices; and develops and improves mechanisms to transfer results of its research to the ultimate user. The Laboratory consists of the following centers:

- Applied Mathematics
- Electronics and Electrical Engineering²
- Manufacturing Engineering
- Building Technology
- Fire Research
- Chemical Engineering³

The Institute for Computer Sciences and Technology

Conducts research and provides scientific and technical services to aid Federal agencies in the selection, acquisition, application, and use of computer technology to improve effectiveness and economy in Government operations in accordance with Public Law 89-306 (40 U.S.C. 759), relevant Executive Orders, and other directives; carries out this mission by managing the Federal Information Processing Standards Program, developing Federal ADP standards guidelines, and managing Federal participation in ADP voluntary standardization activities; provides scientific and technological advisory services and assistance to Federal agencies; and provides the technical foundation for computer-related policies of the Federal Government. The Institute consists of the following divisions:

- Information Systems Engineering
- Systems and Software Technology
- Computer Security
- Systems and Network Architecture
- Advanced Computer Systems

The Institute for Materials Science and Engineering

Conducts research and provides measurements, data, standards, reference materials, quantitative understanding and other technical information fundamental to the processing, structure, properties and performance of materials; addresses the scientific basis for new advanced materials technologies; plans research around cross-cutting scientific themes such as nondestructive evaluation and phase diagram development; oversees Bureau-wide technical programs in nuclear reactor radiation research and nondestructive evaluation; and broadly disseminates generic technical information resulting from its programs. The Institute consists of the following Divisions:

- Ceramics
- Fracture and Deformation³
- Polymers
- Metallurgy
- Reactor Radiation

¹Headquarters and Laboratories at Gaithersburg, MD, unless otherwise noted; mailing address Gaithersburg, MD 20899.

²Some divisions within the center are located at Boulder, CO 80303.

³Located at Boulder, CO, with some elements at Gaithersburg, MD

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET (See instructions)	1. PUBLICATION OR REPORT NO. NBS/TN-1308	2. Performing Organ. Report No. 888 1100514S	3. Publication Date April 1987
4. TITLE AND SUBTITLE NO ₂ Heterodyne Frequency Measurements With a Tunable Diode Laser, A CO Laser Transfer Oscillator, and CO ₂ Laser Standards			
5. AUTHOR(S) L. R. Zink, M. Vanek, and J. S. Wells			
6. PERFORMING ORGANIZATION (If joint or other than NBS, see instructions) NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		7. Contract/Grant No. 8. Type of Report & Period Covered	
9. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS (Street, City, State, ZIP) Supported in part by Upper Atmospheric Research Officer NASA NBS Category No. NBS. 870			
10. SUPPLEMENTARY NOTES <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.			
11. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here) Heterodyne frequency measurements have been made on selected groups of nitrogen dioxide rovibronic transitions between 1580.8 and 1650.7 cm ⁻¹ . The groups are separated by 7 to 10 cm ⁻¹ , and the intent is to provide a limited (and interim) calibration table for the region. In addition to a table of measured frequencies in this region, we have included figures of spectra in the vicinity of the measured lines to provide a map for identifying the transitions measured.			
12. KEY WORDS (Six to twelve entries; alphabetical order; capitalize only proper names; and separate key words by semicolons) calibration frequencies at 6.2 μm; heterodyne frequency measurements; nitrogen dioxide spectra			
13. AVAILABILITY <input checked="" type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS Order From Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402. <input type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA. 22161		14. NO. OF PRINTED PAGES 28 15. Price PC \$11.95	

NO₂ Heterodyne Frequency Measurements With a Tunable Diode Laser, a CO Laser Transfer Oscillator, and CO₂ Laser Standards

**L.R. Zink
M. Vanek
J.S. Wells**

**Time and Frequency Division
Center for Basic Standards
National Measurement Laboratory
National Bureau of Standards
Boulder, Colorado 80303-3328**

**Supported in part by
Upper Atmospheric Research Office
NASA**



U.S. DEPARTMENT OF COMMERCE, Malcolm Baldrige, Secretary

NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Director

Issued April 1987

National Bureau of Standards Technical Note 1308
Natl. Bur. Stand. (U.S.), Tech Note 1308, 28 pages (Apr. 1987)
CODEN:NBTNAE

U.S. GOVERNMENT PRINTING OFFICE
WASHINGTON: 1987

CONTENTS

ABSTRACT	1
INTRODUCTION.....	1
EXPERIMENTAL TECHNIQUES.....	4
CONCLUSION.....	6
ACKNOWLEDGMENT	6
REFERENCES.....	7
APPENDIX.....	10

NO₂ HETERODYNE FREQUENCY MEASUREMENTS WITH A TUNABLE DIODE LASER,
A CO LASER TRANSFER OSCILLATOR, AND CO₂ LASER STANDARDS

L. R. Zink, M. Vanek, and J. S. Wells
Time and Frequency Division
National Bureau of Standards
Boulder, Colorado 80303

Heterodyne frequency measurements have been made on selected groups of nitrogen dioxide rovibronic transitions between 1580.8 and 1650.7 cm⁻¹. The groups are separated by 7 to 10 cm⁻¹, and the intent is to provide a limited (and interim) calibration table for the region. In addition to a table of measured frequencies in this region, we have included figures of spectra in the vicinity of the measured lines to provide a map for identifying the transitions measured.

Key words: calibration frequencies at 6.2 μ m, heterodyne frequency measurements, nitrogen dioxide spectra.

INTRODUCTION

A program was established several years ago to provide reference frequencies for the use of spectroscopists for the calibration of spectra. The objectives at the initiation of the program (with particular emphasis on the use of tunable diode lasers) were to select molecules meeting certain criterion such as

1. Absorption type standards
2. A marker every 0.5 cm⁻¹ (to match TDL mode tunability)
3. A convenient molecule (one easily handled)
4. A simple Hamiltonian
5. Line positions should be good to ± 3 MHz.

The last criterion requires heterodyne frequency measurements and that has been a major task along with the selection and fitting of the best available measurements from the literature. Some of the better candidates were carbonyl sulfide (OCS) and nitrous oxide (N₂O). A large body of work has been completed on OCS [1-5]. OCS has a fairly high abundance of isotopic species which help provide a definite signature (spectroscopic pattern) in the vicinity of a particular calibration feature. A 6600 entry OCS atlas [6],

which gives the transition wavenumber, the transition frequency, the isotopic species, the transition band, the J-value for the transition, the lower state energy level and the intensity in a normal mixture for each line is available. The coverage afforded by OCS shown in figure 1 below.

INFRARED FREQUENCY CALIBRATION STANDARDS

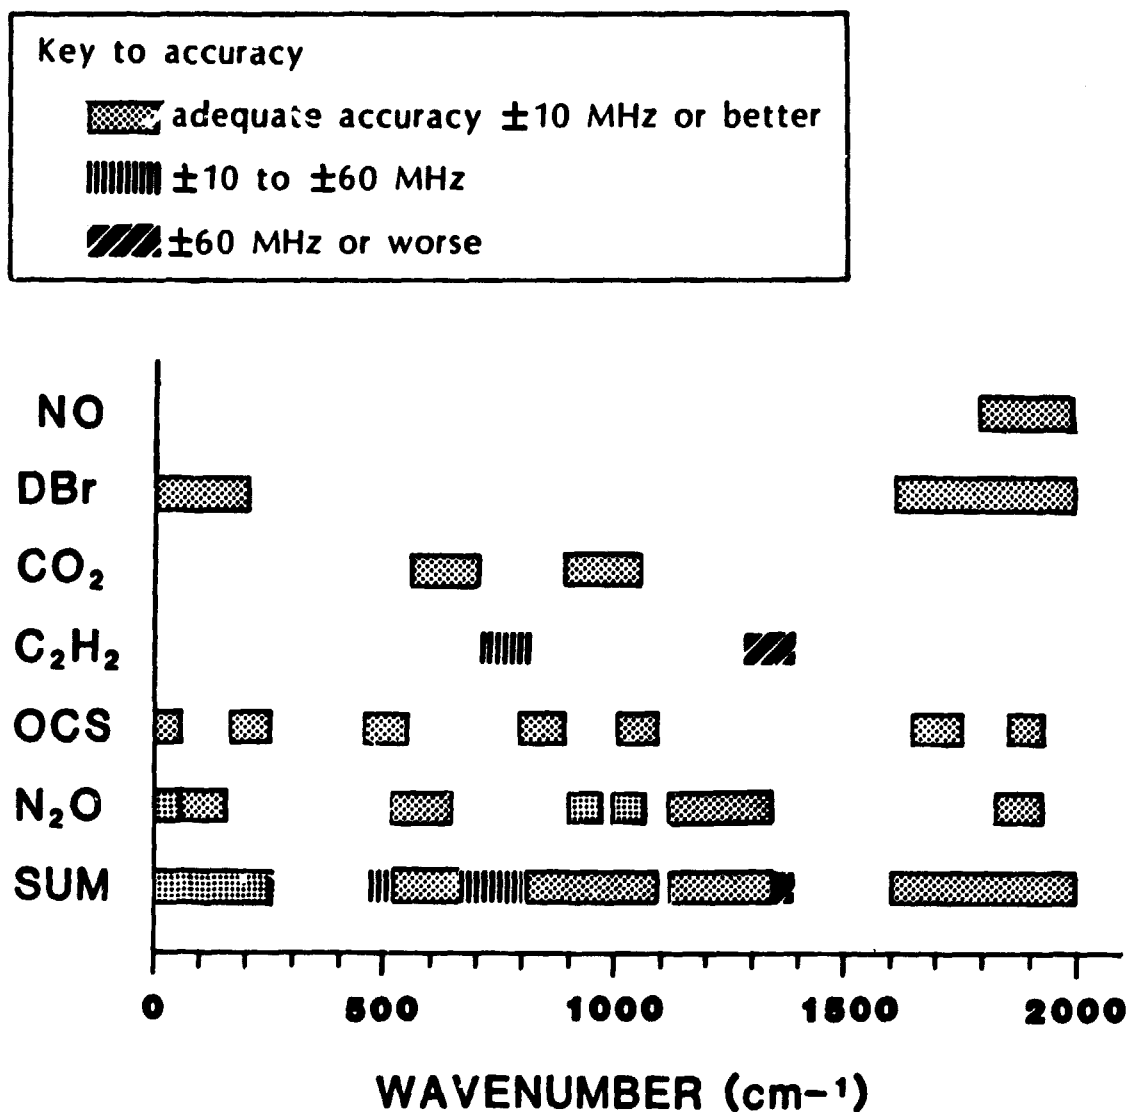


Fig. 1. Accuracy of frequency calibration tables for selected molecules in the 0-2000 cm^{-1} region.

Another prominent molecule in figure 1 is nitrous oxide and a large amount of work has been completed on this molecule [7-9]. An interim calibration table exists for the 8 μm region but more work is needed and has been planned for the future.

While these two molecules satisfy the five criteria above, there are regions of the spectrum where these two molecules leave gaps in the coverage. For example DBr covers some of the gap at 1800 cm^{-1} [10], but it does not meet criterion #2. In DBr the spacing between calibration points is about 10 cm^{-1} and then only two markers appear (separated by about 0.2 cm^{-1}) before another 10 cm^{-1} gap. Nonetheless, users have reported this to be quite useful.

The emphasis of the current work is to address the gap at 1500 cm^{-1} in figure 1 and to provide references similar to that afforded by DBr. In particular, we chose to provide markers every 7 to 10 cm^{-1} and also provide a tunable diode laser (TDL) spectrum of the other lines in the vicinity to serve as a signature.

Nitrogen dioxide does not meet the fourth criterion in that it is an asymmetric rotor with spin split states and its Hamiltonian requires about 25 constants. Further, more than 3000 lines exist in the current Air Force Geophysical Labs (AFGL) tables, and only one or two percent of these are candidates for a heterodyne frequency measurement. Thus, our approach will serve two purposes. First, it will provide frequency measurement based calibration points with strongly absorbing lines in the gap region and serve as an interim calibration table. Second, our past experience with data from different techniques indicates that while Fourier transform spectroscopic (FTS) data are quite satisfactory for some requirements, there can sometimes be a small calibration error. We suggest that the results from our study either will be useful for the calibration of NO_2 in a FTS study, or serve as an independent check of that work. We think that a measurement every 10 cm^{-1} or so will be satisfactory for this purpose. Figure 2 on the next page shows a compressed FTS spectrum of nitrogen dioxide (the intense lines outside the familiar P and R branch structure are H_2O lines) and the position of CO laser lines which were used to make the heterodyne frequency measurements.

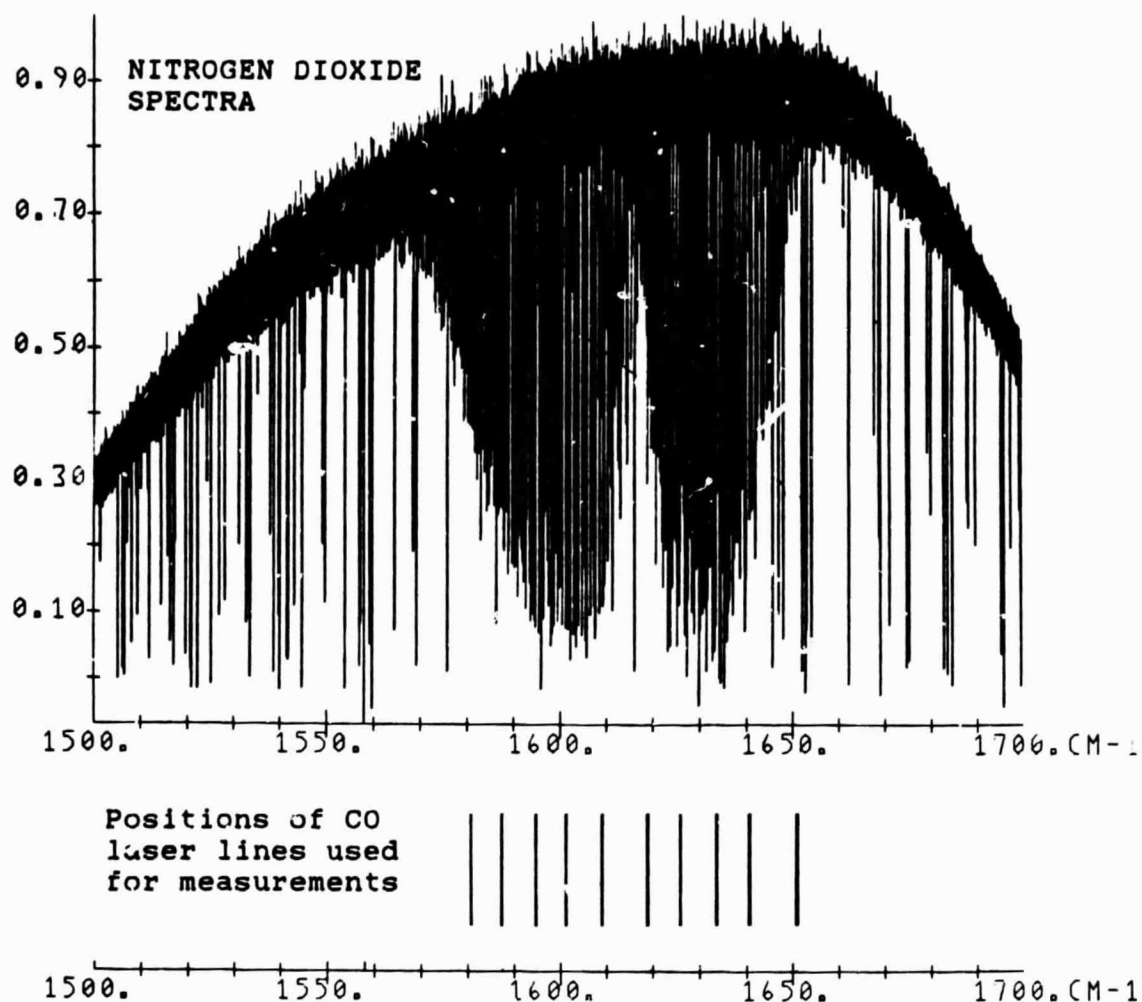


Fig. 2. Overlap between nitrogen dioxide spectra and selected CO laser lines.

EXPERIMENTAL TECHNIQUES

The measurement technique used for these measurements requires the use of a CO laser to act as a transfer oscillator. Its role is to transfer the frequency synthesized from CO₂ laser frequency standards to the frequency of the molecular feature of interest. Each of the frequency measurements of a

nitrogen dioxide transition listed in Table I is a combination of two nearly simultaneous measurements. The first one is a determination of the frequency of a CO laser transition relative to the CO₂ laser standards. By the use of two stabilized CO₂ lasers, a metal-insulator-metal diode, and a microwave oscillator, we generate a frequency, ν_s , given by

$$\nu_s = l\nu_1 + m\nu_2 + n\nu_M, \quad (1)$$

where ν_1 and ν_2 are the frequencies of the CO₂ laser standards, and ν_M is a microwave frequency. The quantities l , m , and n are integers which are allowed both positive and negative values. For these experiments, the value l was always 3, and m was -1. The microwave frequencies are listed in Table I, and the n value may be inferred since an X-band klystron was used. An rf beat note ν_{B1} (the difference between the frequency ν_s and the CO laser frequency ν_{CO}) was taken from the MIM diode, amplified and displayed on an rf spectrum analyzer where its center frequency was marked by an rf synthesizer. The frequency of the transfer oscillator was then

$$\nu_{CO} = \nu_{\text{transfer}} - \nu_s \pm \nu_{B1}. \quad (2)$$

The second part of the measurement was a difference frequency measurement between the CO laser transfer oscillator and a tunable diode laser whose frequency was locked to the NO₂ absorption feature of interest. This difference frequency beat note ν_{B2} had its center frequency marked by a marker oscillator whose frequency was counted and the frequency of the NO₂ transition was then

$$\nu_{\text{NO}_2} = \nu_{\text{transfer}} + \nu_{B2}. \quad (3)$$

The measurements are given in Table I, which gives the CO₂ transitions and the microwave frequency (in some cases a second harmonic is the value shown) involved in each measurement, the frequency of the NO₂ transition along with our estimated uncertainty and finally the quantum numbers assigned are those taken from the AFGL tapes.

Tunable diode laser spectra in the vicinity of each of the CO laser lines used for the measurements are given in the appendix. These were observed at a pressure of 113 Pa and a path length of 1.7 m. Differences between the calculated frequency values in the AFGL tables and our heterodyne measurements range from a few megahertz up to hundreds of megahertz for some transitions.

For the heterodyne frequency measurements in Table I, the path length was also 1.7 m. The pressure was reduced so that for each transition measured the absorption was in the linear regime. Typically, these pressures were in the 50 to 100 Pa range.

CONCLUSION

Since NO_2 is an asymmetric rotor with spin split states and the majority of the more than 3000 lines given in the AFGL tables are not close enough to CO laser lines to permit heterodyne frequency measurements on them, we believe the better approach is to measure only enough lines for the calibration and leave the detailed spectra for a FTS study. This will permit us to use our resources to look at some N_2O hot band features in the 1600 cm^{-1} region. This represents something of a trade-off; a long path cell will be required for the N_2O spectra, but a marker every 0.5 cm^{-1} should be available. The greater absorption afforded by NO_2 will permit its use by all, but until a more detailed study with a high resolution FTS instrument such as that accessible to the JPL is complete, only a limited number of reference points will be available.

ACKNOWLEDGMENT

We would like to thank Dr. J. Burkholder for taking some preliminary FTS data on the local Bomen instrument of NOAA at our request. We also thank Dr. D. A. Jennings for the use of his frequency synthesis programs. We are grateful to Dr. A. Maki for his continuing cooperation and advice regarding our frequency standards program. This work was supported in part by the Upper Atmospheric Research Office of NASA.

REFERENCES

- [1] Heterodyne Frequency Measurements with a Tunable Diode Laser CO₂ Laser Spectrometer: Spectroscopic Reference Frequencies in the 9.5 μ m Band of Carbonyl Sulfide, J.S. Wells, F.R. Petersen and A.G. Maki, Appl. Opt. 18, 3567-3573 (1979).
- [2] Heterodyne Frequency Measurements on the 11.6 μ m Band of Carbonyl Sulfide (OCS) and New Frequency/Wavelength Calibration Tables for both the 11.6 and 5.8 μ m OCS Bands, Appl. Opt. 20, 1676-1684 (1980). Erratum: Appl. Opt. 20, 2874 (1981).
- [3] Heterodyne Frequency Measurements (at 11.6 μ m) on Isotopic Species of Carbonyl Sulfide, OC³⁴S, O¹³CS, OC³³S, ¹⁸OCS, and O¹³C³⁴S, J.S. Wells, F.R. Petersen, A.G. Maki, and D.J. Sukle, J. Mol. Spectrosc. 89, 421-429 (1981).
- [4] Heterodyne Frequency Measurements of Carbonyl Sulfide Transitions at 26 and 51 THz; Improved OCS, O¹³CS, and OC³⁴S Molecular Constants, J.S. Wells, F.R. Petersen and A.G. Maki, J. Mol. Spectrosc. 98, 404-412 (1983).
- [5] Heterodyne Frequency Measurements on the 12⁰0-00⁰0 Band of OCS, A.G. Maki, J.S. Wells, and A. Hinz, Int'l J. IR & MM Waves, 7, 909-917 (1986).
- [6] Tables of Carbonyl Sulfide (OCS) Absorption Line Frequencies and Wave-numbers for the Calibration of Tunable Infrared Lasers, A.G. Maki, J.S. Wells, F.R. Petersen, W.J. Lafferty, W.B. Olson, A. Fayt, and J.P. Sattler, J. Phys. Chem. Ref. Data (in process).
- [7] Absolute Frequency Measurements of the 00⁰2-00⁰0, 20⁰1-00⁰0, and 12⁰1-00⁰ Bands of N₂O by Heterodyne Spectroscopy, C.R. Pollock, F.R. Petersen, D.A. Jennings, J.S. Wells, and A.G. Maki, J. Mol. Spectrosc. 107, 62-71 (1984).
- [8] Heterodyne Frequency Measurements on N₂O at 5.3 and 9.0 μ m, J.S. Wells, D.A. Jennings, A. Hinz, J.S. Murray, and A.G. Maki, J. Opt. Soc. Am. B2, 857-861 (1985).
- [9] Heterodyne Frequency Measurements on the 10⁰0-00⁰0 Band of N₂O Near 8 μ m, J.S. Wells, A. Hinz, and A.G. Maki, J. Mol. Spectrosc. 114, 84-96 (1985).
- [10] Heterodyne Measurements of Hot Bands and Isotopic Transitions of N₂O near

1300 cm^{-1} , A. Hinz, J.S. Wells, and A.G. Maki, Atoms, Molecules, and Clusters, (in press).

- [11] Improved Deuterium Bromide 1-0 Band Molecular Constants from Heterodyne Frequency Measurements, J.S. Wells, D.A. Jennings, and A.G. Maki, J. Mol. Spectrosc. 107, 48-61 (1984).

APPENDIX

This appendix contains ten figures of nitrogen dioxide spectra in the vicinity of the CO laser lines which were used in the heterodyne frequency measurements. We have included them because we found the lower resolution AFGL data to be somewhat difficult to reconcile with the higher resolution TDL spectra. In some cases, this may have been due to less accurate line position data (calculated values in error due to poor constants) for example. In other cases, perhaps it was simply a resolution problem. In any case, we have found it preferable to have a signature at the resolution attainable by the instrument at hand and, given the current status of the data (numerical data not available at accuracy reported here), we feel spectral samples are the interim answer.

Most of the spectra were recorded at a pressure of 113 Pa (0.85 torr) in an absorption cell 1.7 m long. For the more intense regions of the spectra, the pressure was reduced for the duration of a particular heterodyne frequency measurement. The pressure was in general reduced to the linear absorption regime and this afforded lines to be resolved that do not appear so in the spectra shown (see Figs. A-4 and A-8 for example).

Three sets of numbers (given in cm^{-1}) appear in the figures. The heterodyne frequency measurements are given in square brackets with the uncertainty in the last digits for the measurement given in parentheses within the bracket, i.e., [1580.73450(33)]. These numbers are positioned on the page so that the decimal point lines up above the center of the line that was measured, and in most cases they are placed above the spectra. A second set of numbers comes from newly taken FTS data; in this case only the numbers to the right of the decimal point are listed, except for a few obvious instances. The FTS numbers are meant to supplement the frequency measurements and are listed in parentheses. In some instances, these have been corrected where a disagreement with heterodyne measurement seems to warrant it. Uncertainties are not given for these measurements, but we believe that the values we list are good to within 0.0005 cm^{-1} . The third set of numbers was taken from the AFGL tables; these are positioned near the NO_2 spectra baseline and consist of only the three significant digits listed in the tables.

Fringes from a 7.5 cm germanium etalon were recorded below the NO₂ spectra. Since the etalon was not temperature stabilized, these should not be relied upon for interpolation. We have used them only for line identification purposes.

Table I. Heterodyne Frequency Measurements on Nitrogen Dioxide with the Aid of a CO Laser Transfer Oscillator.

Synthesis Scheme			CO laser	NO ₂ Transition								
CO ₂ trans. for 3v ₁	CO ₂ trans. for -v ₂	MW freq. MHz	trans. P _{v''} (J'')	Frequency ^a MHz	Quantum Numbers							
					J'	K _a '	Kc'	J''	K _a ''	Kc''	S-St	
I636 ^b P 22	II626 P 32	24 200	P ₁₇ (15)	49488134.4(90)	49	0	49	48	0	48	+	
I636 P 18	II626 P 10	11 600	P ₁₈ (11)	49190236.8(70)	37	4	33	36	4	32	-	
				49190087.6(70)	37	4	33	36	4	32	+	
I636 P 24	II626 P 20	7 500	P ₁₈ (13)	48973387.0(70)	22	1	22	21	1	21	-	
				48971356.7(90)	24	3	22	23	3	21	-	
				48971185.8(90)	24	3	22	23	3	21	+	
				48967881.8(70)	26	4	23	25	4	22	-	
				48967623.7(70)	26	4	23	25	4	22	+	
I636 P 24	II626 P 12	0	P ₁₈ (15)	48758099.8(70)	19	5	14	18	5	13	-	
				48752991.2(70)	22	6	17	21	6	16	-	
				48749412.1(70)	14	3	12	13	3	11	-	
				48748404.3(70)	16	4	13	15	4	12	+	
I636 P 18	II626 R 16	-11 000	P ₁₉ (10)	48555023.3(70)	21	8	13	20	8	12	+	
				48551625.6(70)	10	5	6	9	5	5	-	
				48550704.5(100)	13	6	7	12	6	6	-	
I636 P 30	II626 P 10	22 000	P ₁₉ (13)	48231914.6(50)	6	6	1	6	6	0	-	
				48231205.7(50)	6	3	4	7	3	5	+	
				48229667.9(50)	7	6	1	7	6	2	+	
				48229360.7(50)	8	6	3	8	6	2	-	
				48228499.0(100)	8	6	3	8	6	2	+	
				48227145.8(100)	9	6	3	9	6	4	+	
				48226313.4(50)	10	6	5	10	6	4	-	
				48225637.6(50)	10	6	5	10	6	4	+	
I636 P 22	II626 R 28	-10 000	P ₂₀ (8)	48023593.6(70)	12	4	9	13	4	10	+	
				48023320.2(70)	12	4	9	13	4	10	-	
				48020088.1(70)	15	2	13	16	2	14	±	
				48019774.1(70)	16	1	16	17	1	17	±	
				48018936.9(70)	10	5	6	11	5	7	+	
				48018294.6(70)	10	5	6	11	5	7	-	
I636 P 36	II626 P 14	10 000	P ₂₀ (10)	47817726.7(100)	21	3	18	22	3	19	±	
I636 P 28	II626 R 24	- 8 800	P ₂₀ (12)	47605993.0(100)	16	8	9	17	8	10	+	
				47605568.1(90)	16	8	9	17	8	10	-	
I636 P 30	II626 R 26	-20 200	P ₂₀ (14)	47394158.7(100)	not assigned							
				47389778.9(100) ^c	32	5	28	33	5	29	±	
				47389452.2(100)	20	9	12	21	9	13	±	
				47389228.2(100)	20	9	12	21	9	13	-	

a) The uncertainty in the last digits is given in parentheses.

b) The notation 626 and 636 refers to the ¹²C¹⁶O₂ and ¹³C¹⁶O₂ isotopic lasers respectively.

c) We estimate that we locate the maximum point of this line to within 10 MHz, however the line is blended, possibly with a water vapor line.

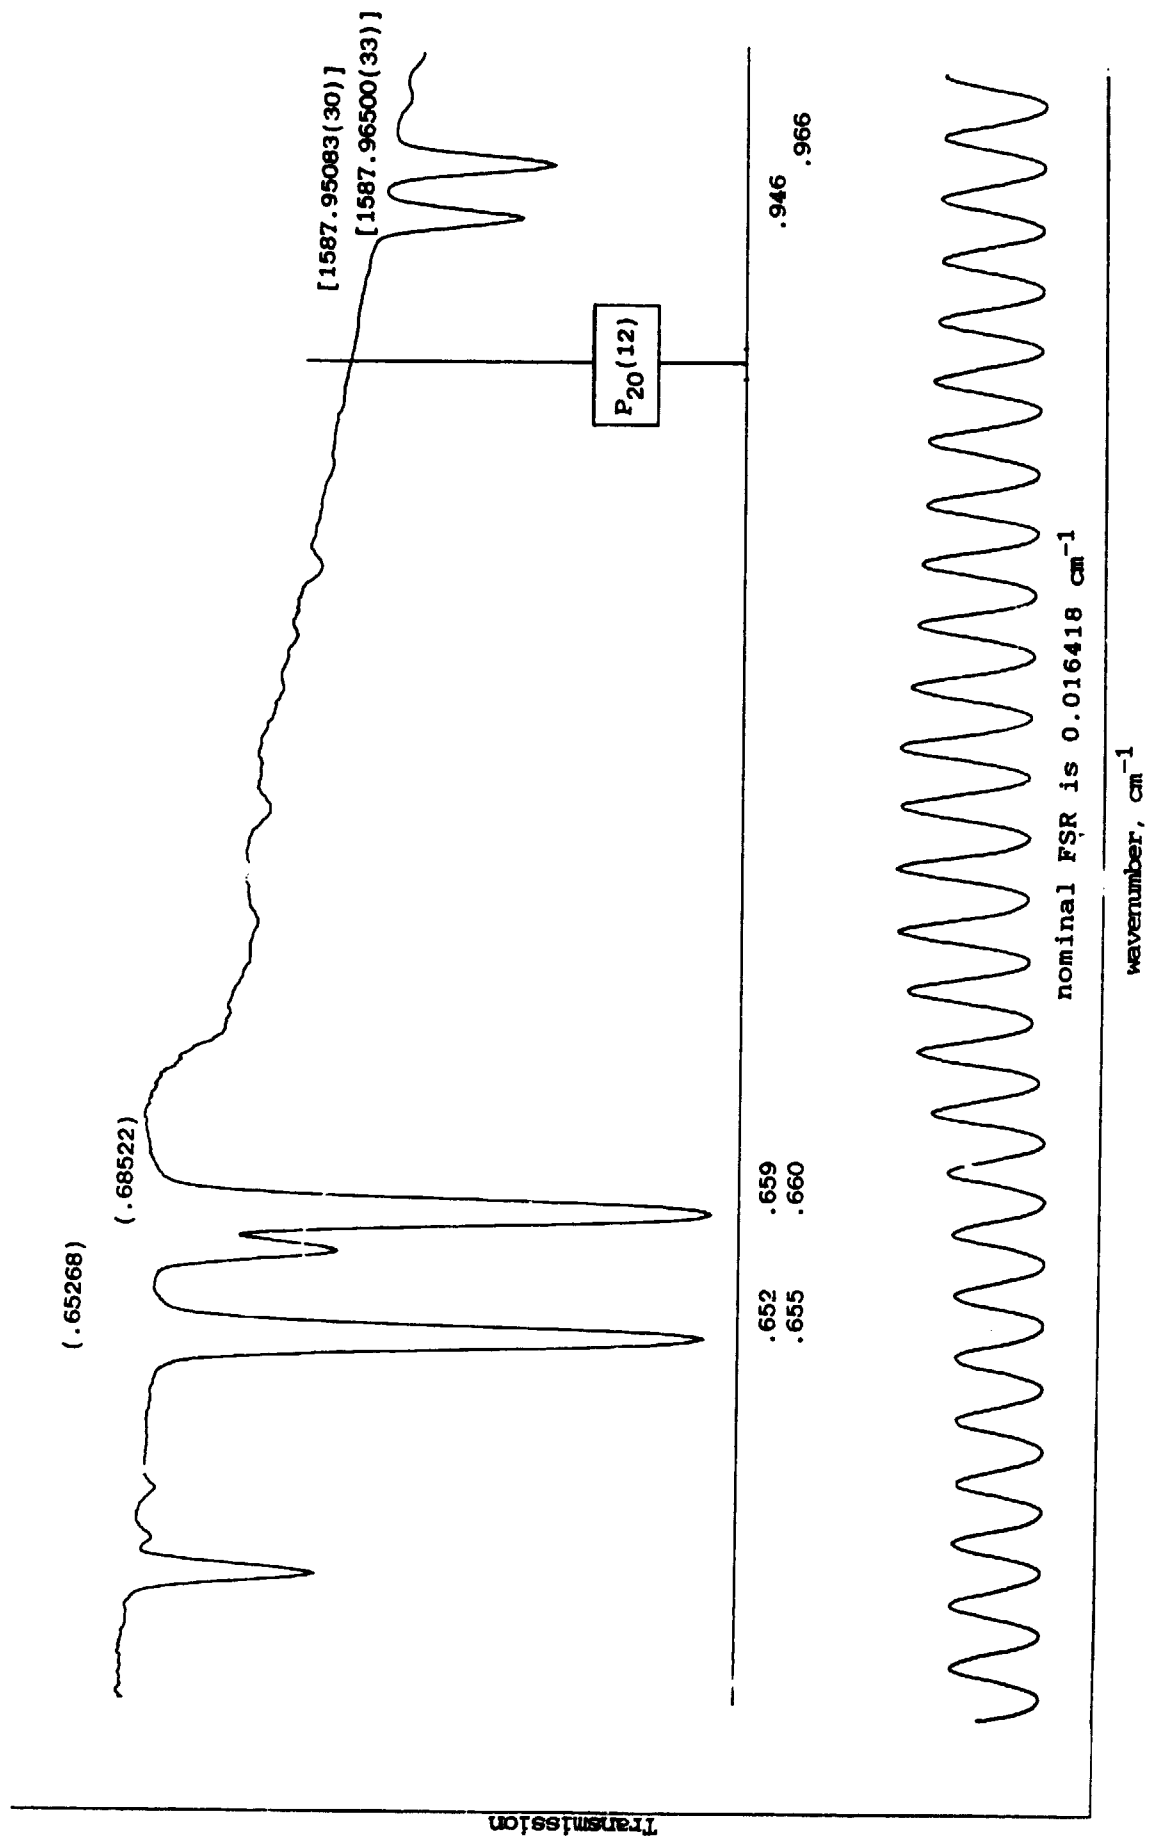


Fig. A-2. Nitrogen dioxide spectra in the vicinity of the $P_{20}(12)$ CO laser line at $1587.91265 \text{ cm}^{-1}$.

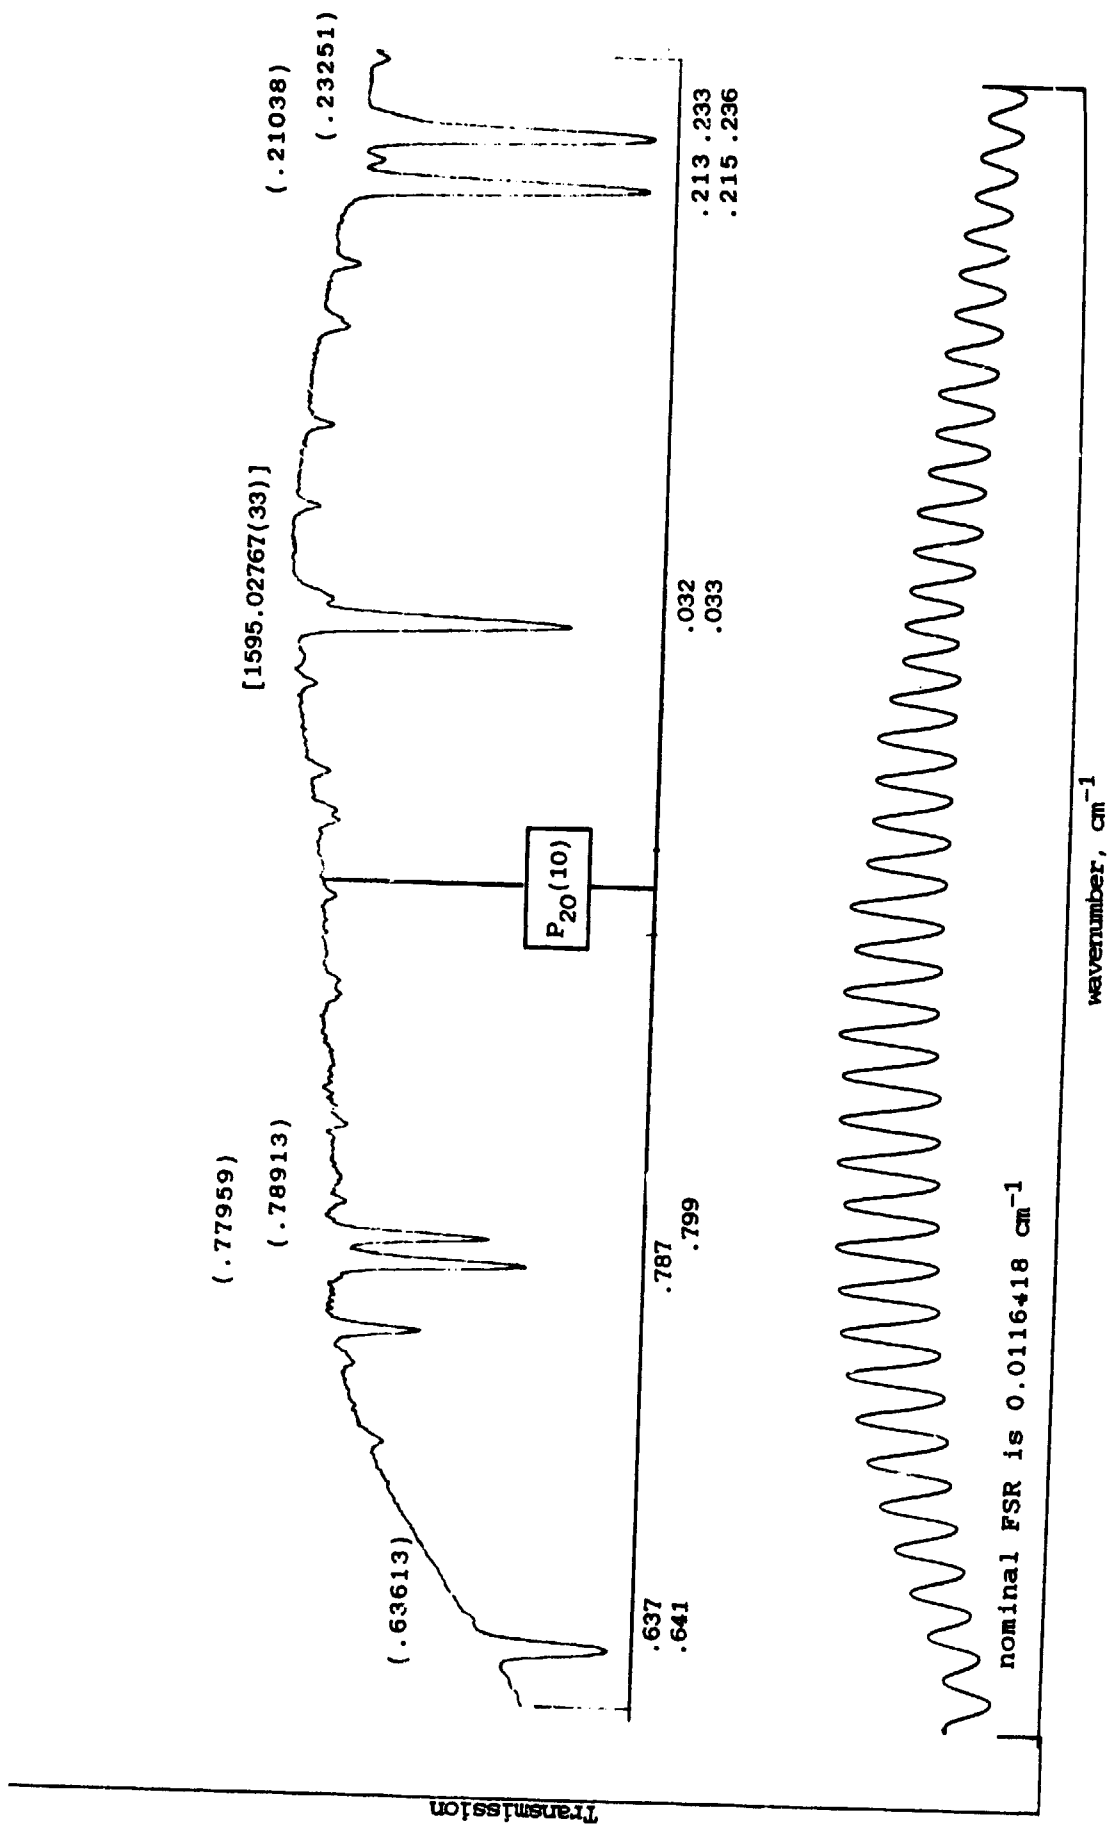


Fig. A-3. Nitrogen dioxide spectra in the vicinity of the $P_{20}(10)$ CO laser line at $1594.91939 \text{ cm}^{-1}$.

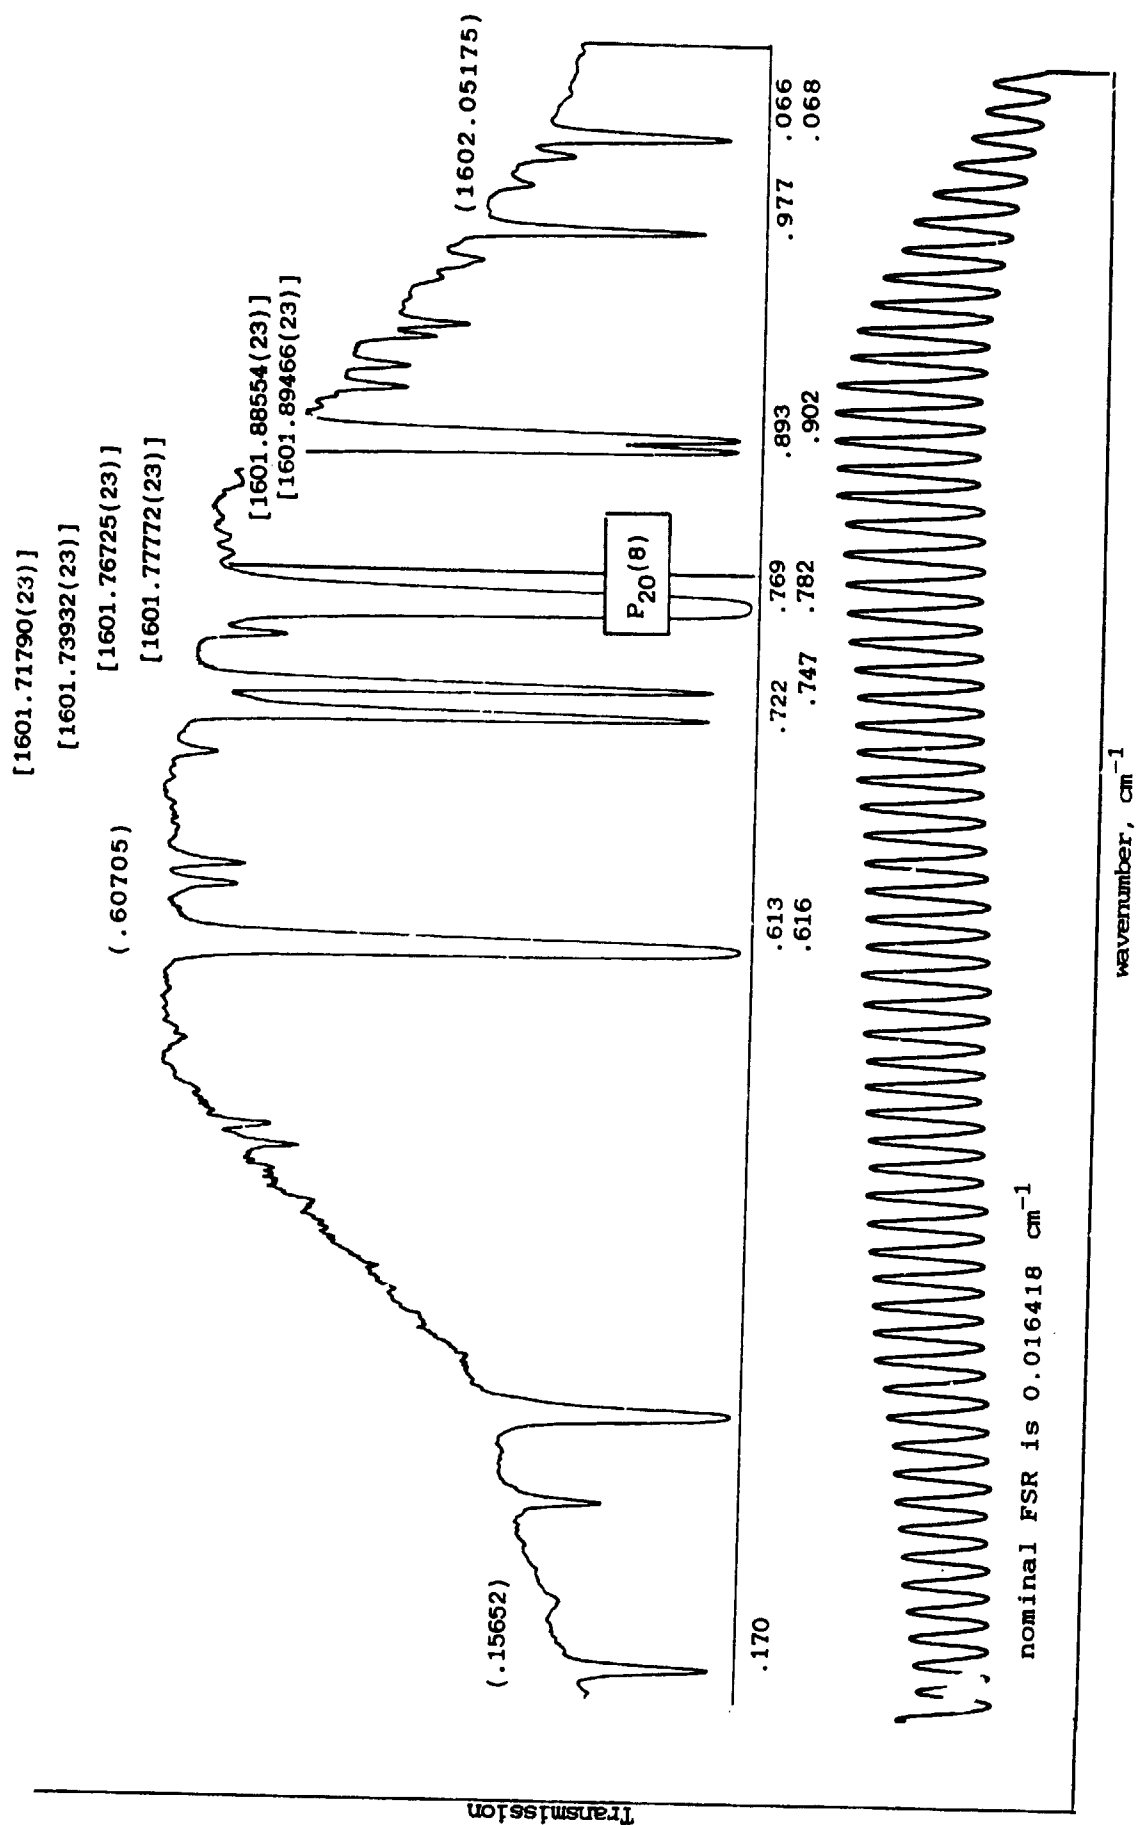


Fig. A-4. Nitrogen dioxide spectra in the vicinity of the $P_{20}(8)$ CO laser line at $1601.79240 \text{ cm}^{-1}$.

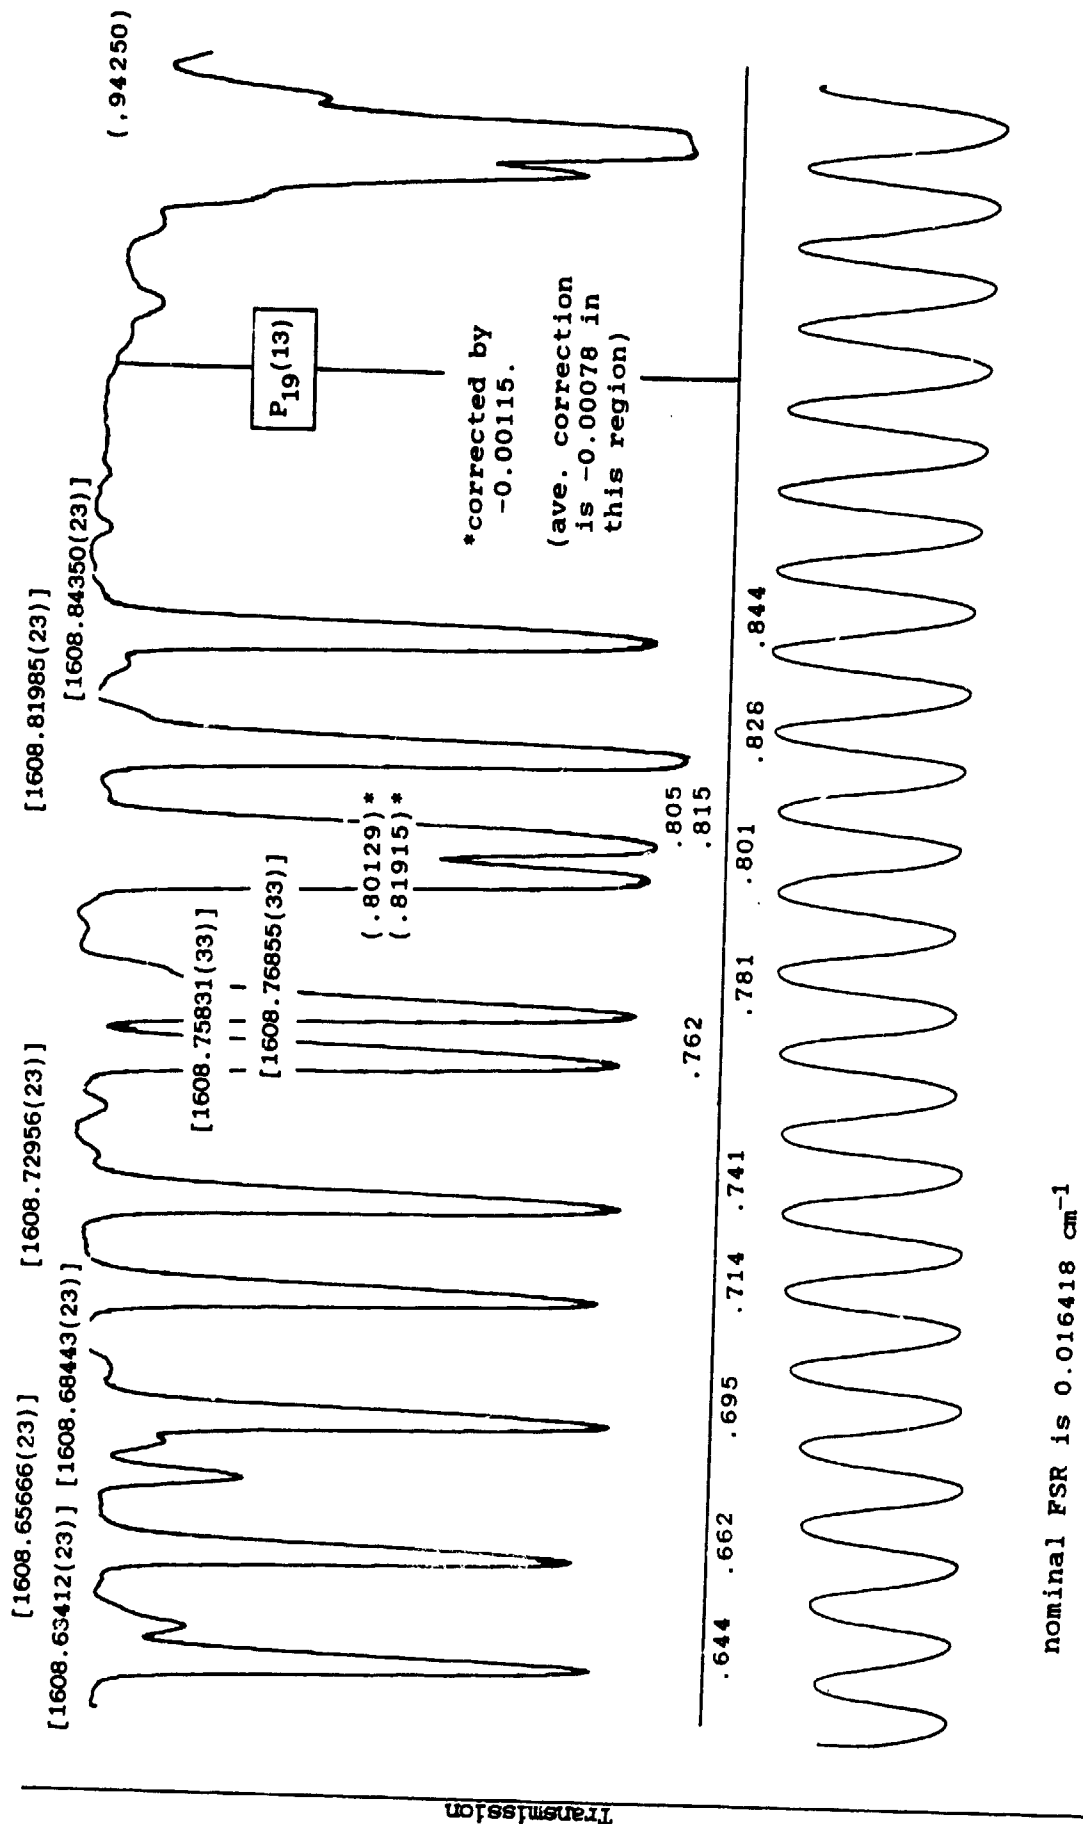


Fig. A-5. Nitrogen dioxide spectra in the vicinity of the $P_{19}(13)$ CO laser line at $1608.89765 \text{ cm}^{-1}$.

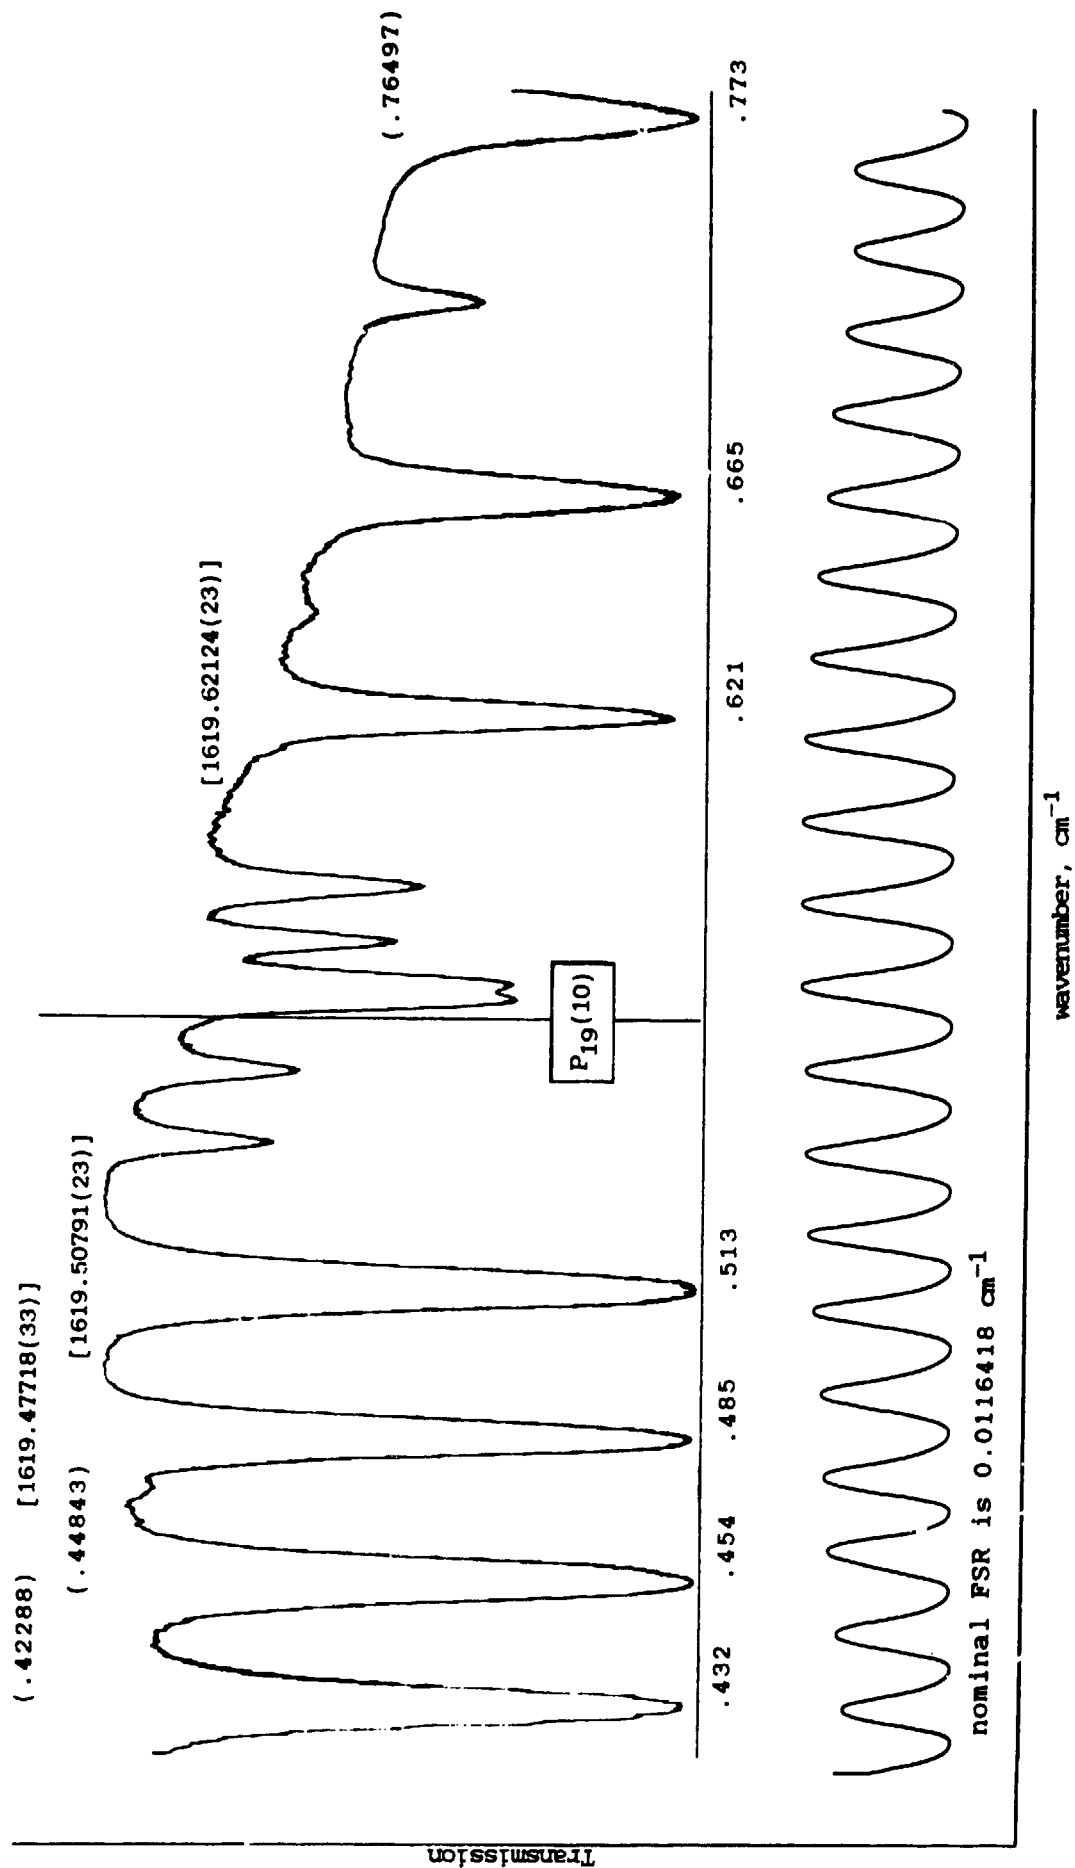


Fig. A-6. Nitrogen dioxide spectra in the vicinity of the P₁₉(10) CO laser line at 1619.56237 cm⁻¹.

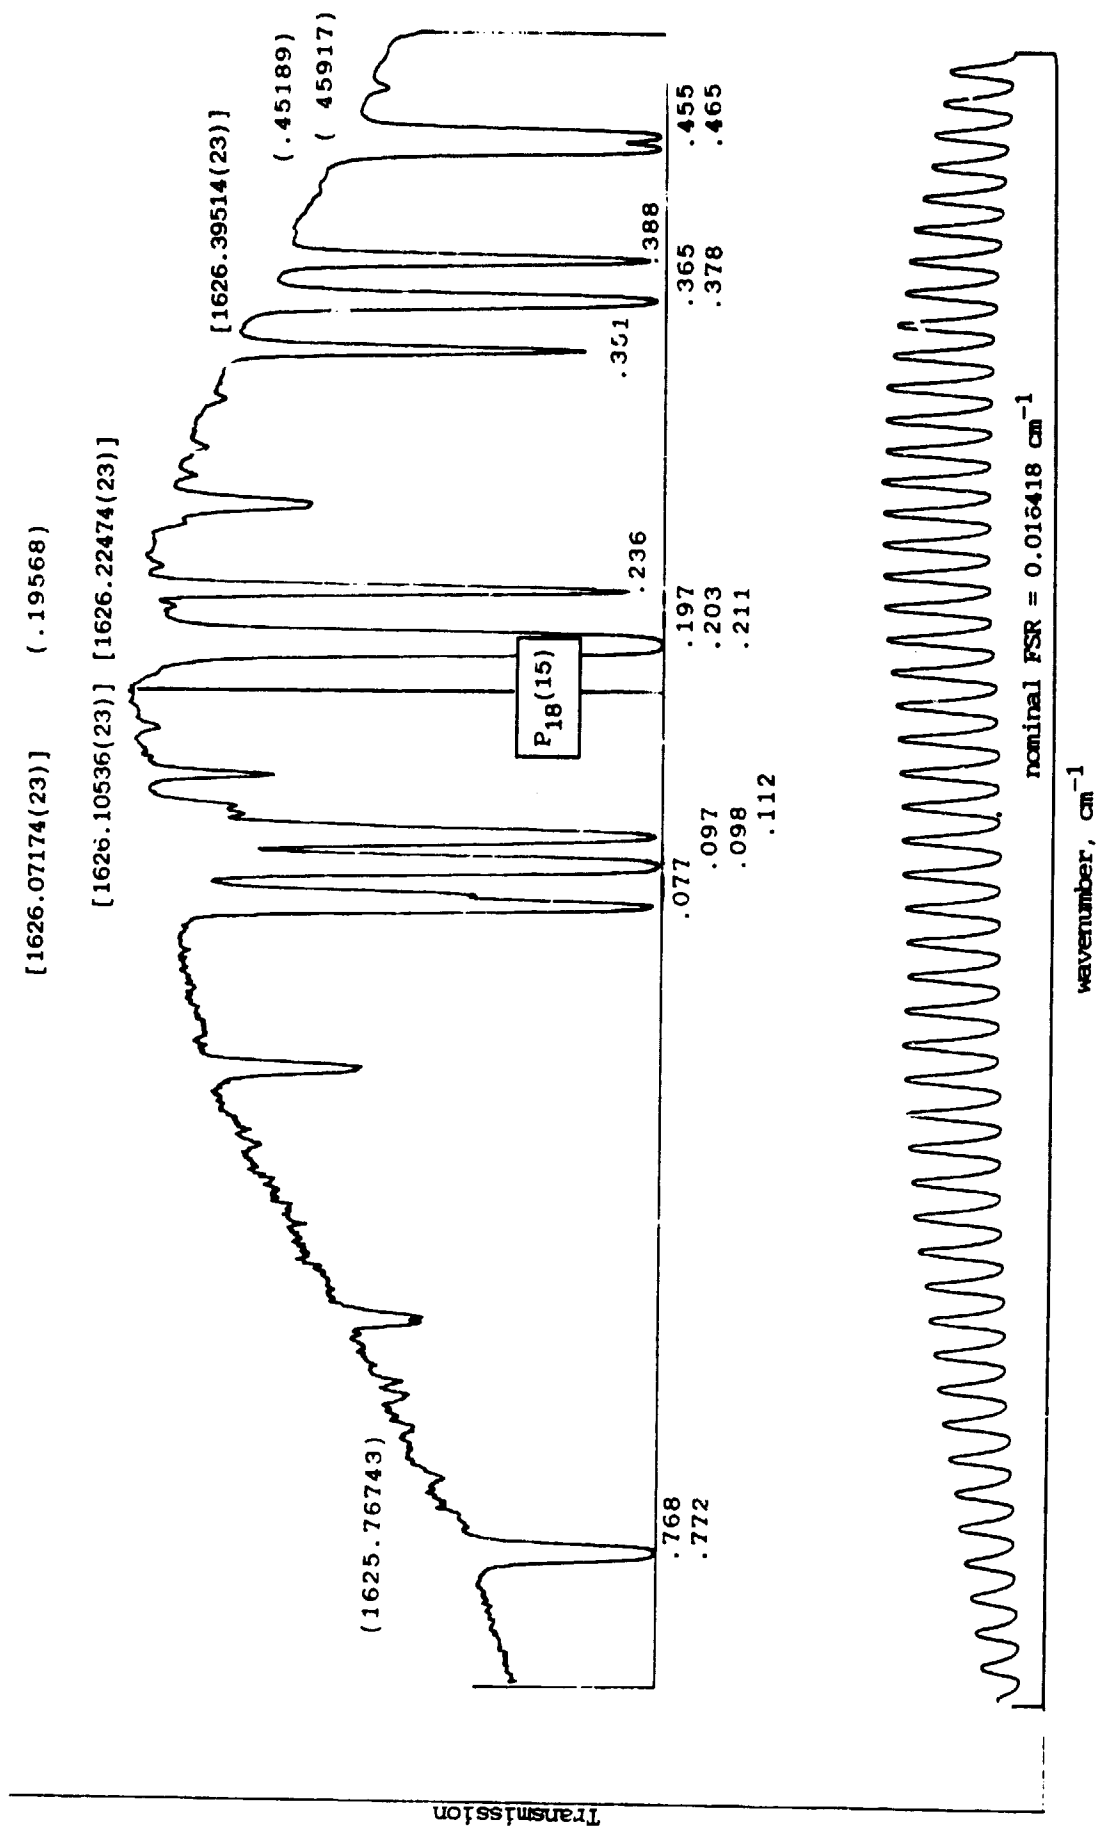


Fig. A-7. Nitrogen dioxide spectrum in the vicinity of the P₁₈(15) CO laser line at 1626.17454 cm⁻¹.

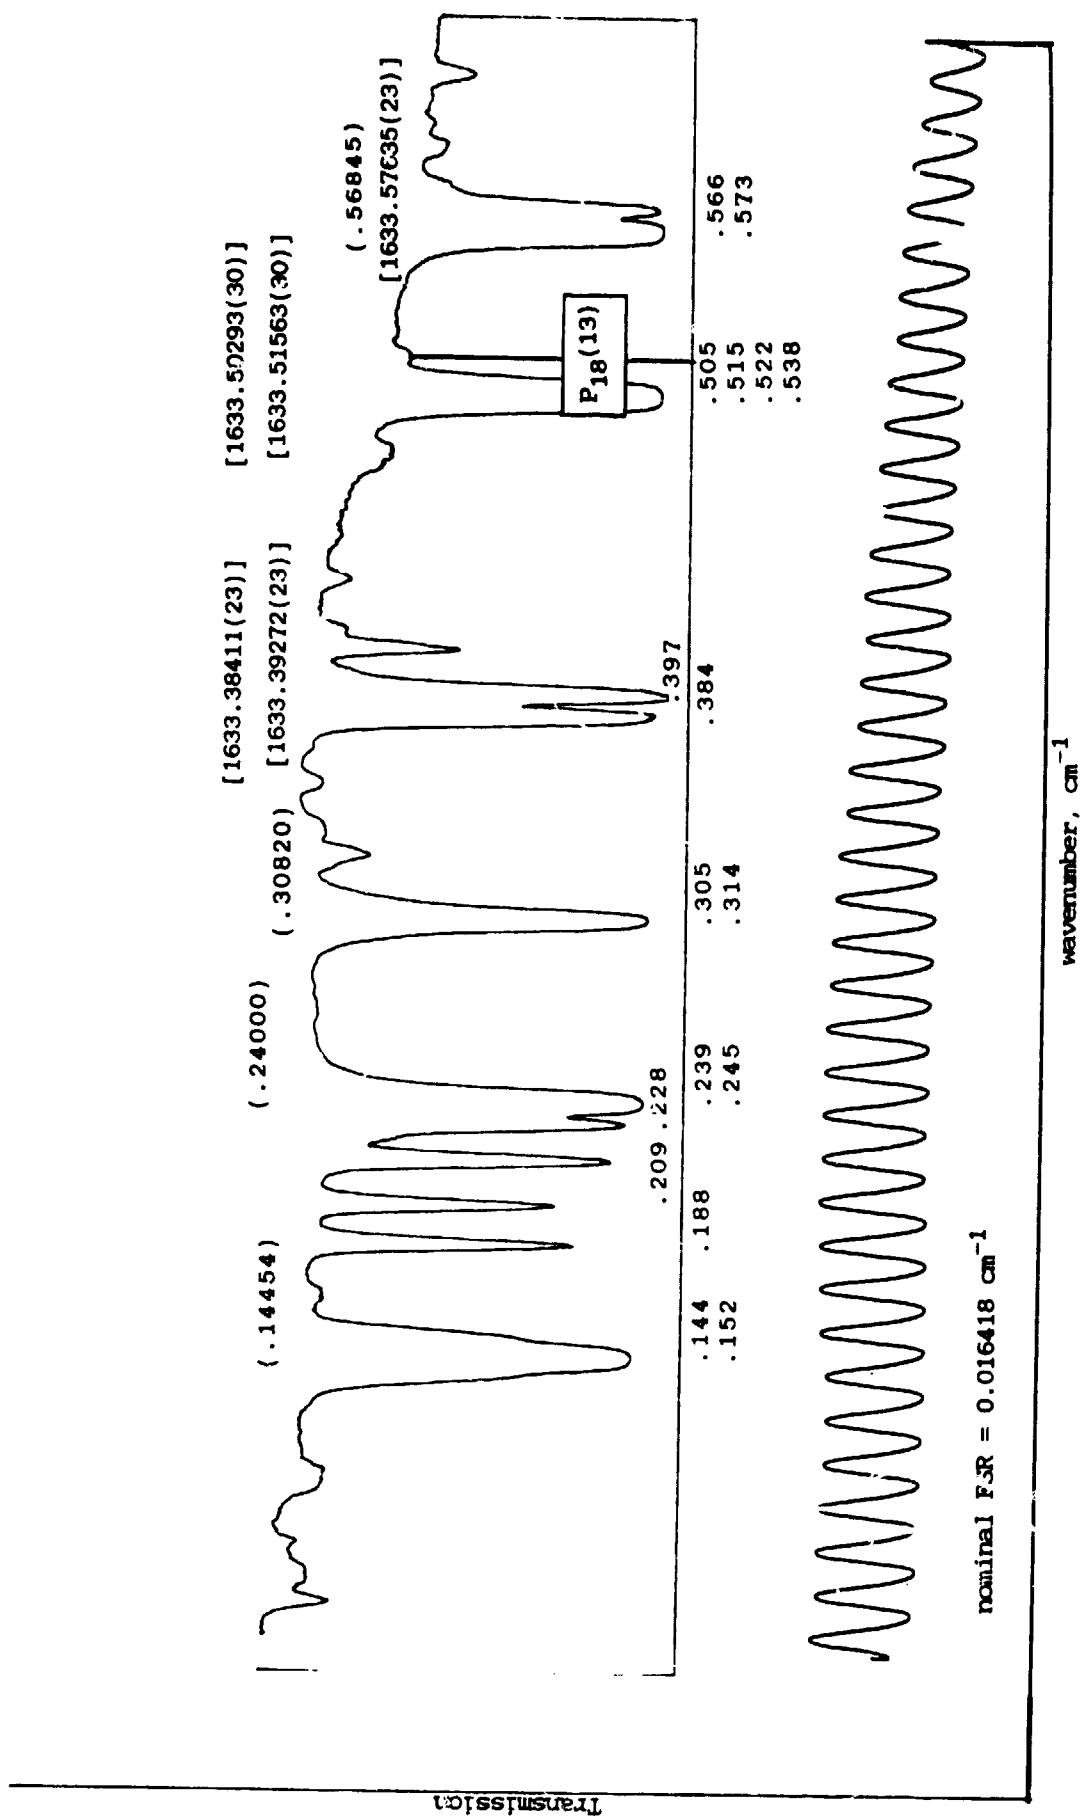


Fig. A-8. Nitrogen dioxide spectra in the vicinity of the P₁₈(13) CO laser line at 1633.51953 cm^{-1} .

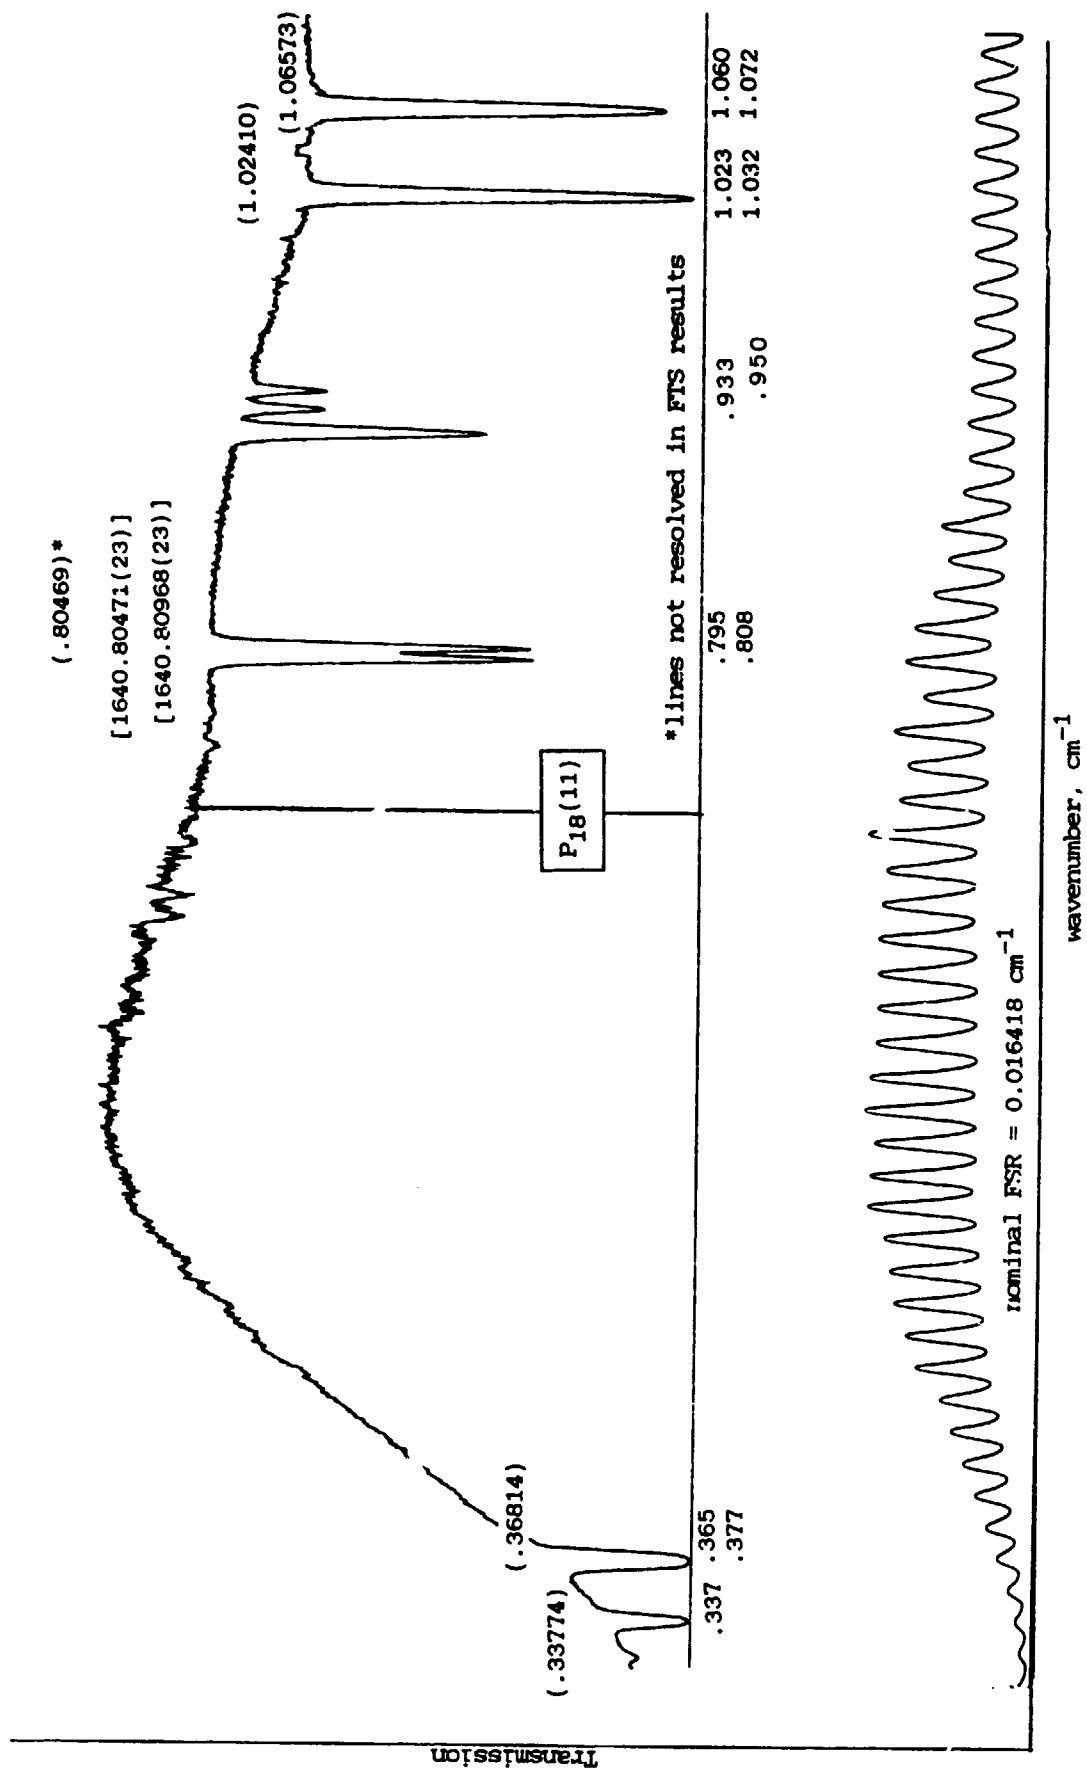


Fig. A-9. Nitrogen dioxide spectra in the vicinity of the P₁₈(11) CO laser line at 1640.73251 cm^{-1} .

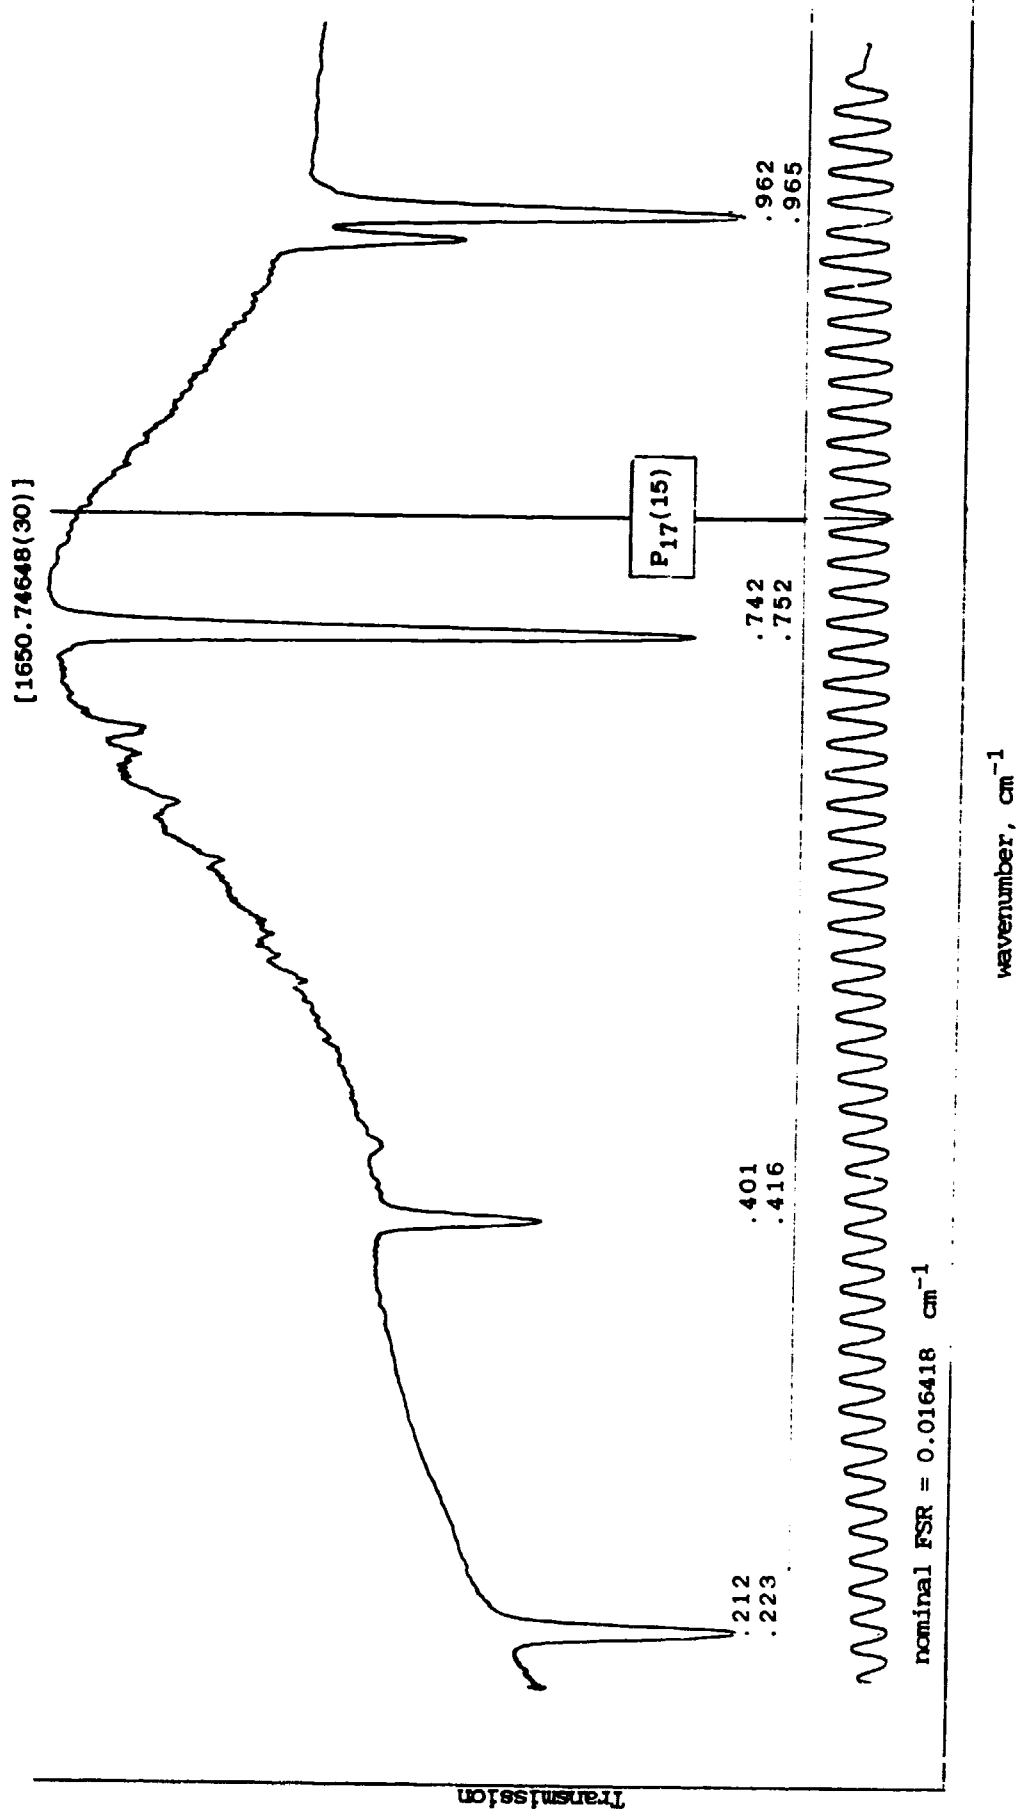


Fig. A-10. Nitrogen dioxide spectra in the vicinity of the $P_{17}(15)$ CO laser line at $1650.81080 \text{ cm}^{-1}$.

NBS *Technical Publications*

Periodical

Journal of Research—The Journal of Research of the National Bureau of Standards reports NBS research and development in those disciplines of the physical and engineering sciences in which the Bureau is active. These include physics, chemistry, engineering, mathematics, and computer sciences. Papers cover a broad range of subjects, with major emphasis on measurement methodology and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Bureau's technical and scientific programs. Issued six times a year.

Nonperiodicals

Monographs—Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

Handbooks—Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

Special Publications—Include proceedings of conferences sponsored by NBS, NBS annual reports, and other special publications appropriate to this grouping such as wall charts, pocket cards, and bibliographies.

Applied Mathematics Series—Mathematical tables, manuals, and studies of special interest to physicists, engineers, chemists, biologists, mathematicians, computer programmers, and others engaged in scientific and technical work.

National Standard Reference Data Series—Provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated. Developed under a worldwide program coordinated by NBS under the authority of the National Standard Data Act (Public Law 90-396).

NOTE: The Journal of Physical and Chemical Reference Data (JPCRD) is published quarterly for NBS by the American Chemical Society (ACS) and the American Institute of Physics (AIP). Subscriptions, reprints, and supplements are available from ACS, 1155 Sixteenth St., NW, Washington, DC 20056.

Building Science Series—Disseminates technical information developed at the Bureau on building materials, components, systems, and whole structures. The series presents research results, test methods, and performance criteria related to the structural and environmental functions and the durability and safety characteristics of building elements and systems.

Technical Notes—Studies or reports which are complete in themselves but restrictive in their treatment of a subject. Analogous to monographs but not so comprehensive in scope or definitive in treatment of the subject area. Often serve as a vehicle for final reports of work performed at NBS under the sponsorship of other government agencies.

Voluntary Product Standards—Developed under procedures published by the Department of Commerce in Part 10, Title 15, of the Code of Federal Regulations. The standards establish nationally recognized requirements for products, and provide all concerned interests with a basis for common understanding of the characteristics of the products. NBS administers this program as a supplement to the activities of the private sector standardizing organizations.

Consumer Information Series—Practical information, based on NBS research and experience, covering areas of interest to the consumer. Easily understandable language and illustrations provide useful background knowledge for shopping in today's technological marketplace.

Order the above NBS publications from: Superintendent of Documents, Government Printing Office, Washington, DC 20402.

Order the following NBS publications—FIPS and NBSIR's—from the National Technical Information Service, Springfield, VA 22161.

Federal Information Processing Standards Publications (FIPS PUB)—Publications in this series collectively constitute the Federal Information Processing Standards Register. The Register serves as the official source of information in the Federal Government regarding standards issued by NBS pursuant to the Federal Property and Administrative Services Act of 1949 as amended, Public Law 89-306 (79 Stat. 1127), and as implemented by Executive Order 11717 (38 FR 12315, dated May 11, 1973) and Part 6 of Title 15 CFR (Code of Federal Regulations).

NBS Interagency Reports (NBSIR)—A special series of interim or final reports on work performed by NBS for outside sponsors (both government and non-government). In general, initial distribution is handled by the sponsor; public distribution is by the National Technical Information Service, Springfield, VA 22161, in paper copy or microfiche form.