

## ABLATION MODELING OF ARES-I UPPER STAGE THERMAL PROTECTION SYSTEM USING THERMAL DESKTOP

John R. Sharp, Arthur T. Page  
 NASA/ Marshall Space Flight Center  
 EV34/Thermal Analysis & Control Branch  
 Huntsville, Alabama

### ABSTRACT:

The thermal protection system (TPS) for the Ares-I Upper Stage will be based on Space Transportation System External Tank (ET) and Solid Rocket Booster (SRB) heritage materials. These TPS materials were qualified via hot gas testing that simulated ascent and re-entry aerothermodynamic convective heating environments. From this data, the recession rates due to ablation were characterized and used in thermal modeling for sizing the thickness required to maintain structural substrate temperatures. At Marshall Space Flight Center (MSFC), the in-house code ABL is currently used to predict TPS ablation and substrate temperatures as a FORTRAN application integrated within SINDA/G. This paper describes a comparison of the new ablation utility in Thermal Desktop and SINDA/FLUINT with the heritage ABL code and empirical test data which serves as the validation of the Thermal Desktop software for use on the design of the Ares-I Upper Stage project.

### INTRODUCTION:

The Ares-I Upper Stage is powered by the J-2X engine, which utilizes Liquid Hydrogen fuel and Liquid Oxygen oxidizer. These large cryogenic tanks are insulated with External Tank (ET) derived polyurethane closed-cell foam, also called Spray-On Foam Insulation (SOFI) to minimize heat leak and ice/frost formation as well maintaining structural temperature limits during ascent aerothermodynamic heating. Various raised areas (protuberances), such as the feed-lines, systems tunnel, reaction control system and solid motor fairings, are insulated with ET and SRB derived TPS materials, such as Super Lightweight Ablator (SLA-561). The primary tool chosen for the in-house Upper Stage thermal design and analysis is Thermal Desktop® (TD) with SINDA/FLUINT. Other software packages are being utilized by MSFC, such as FEMAP, SINDA/G and PATRAN, but the baseline tool for integrated modeling and the bulk of the component

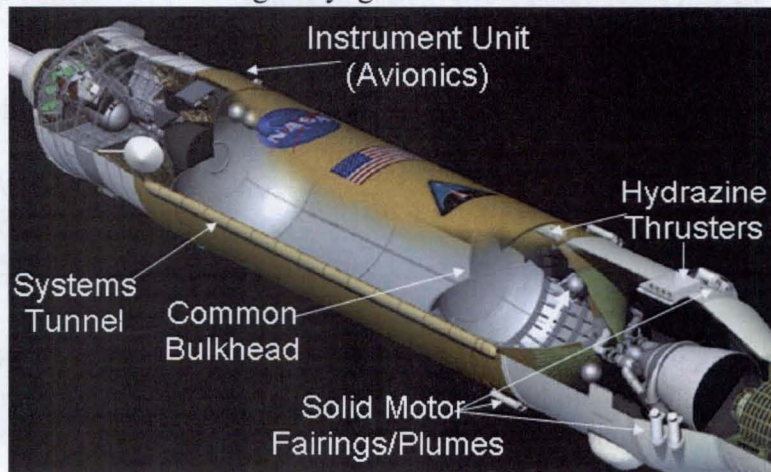


Figure 1: Ares I Upper Stage Overview

The Ares-I Upper Stage is powered by the J-2X engine, which utilizes Liquid Hydrogen fuel and Liquid Oxygen oxidizer. These large cryogenic tanks are insulated with External Tank (ET) derived polyurethane closed-cell foam, also called Spray-On Foam Insulation (SOFI) to minimize heat leak and ice/frost formation as well maintaining structural temperature limits during ascent aerothermodynamic heating. Various raised areas (protuberances), such as the feed-lines, systems tunnel, reaction control system and solid motor fairings, are insulated with ET and SRB derived TPS materials, such as Super Lightweight Ablator (SLA-561). The primary tool chosen for the in-house Upper Stage thermal design and analysis is Thermal Desktop® (TD) with SINDA/FLUINT. Other software packages are being utilized by MSFC, such as FEMAP, SINDA/G and PATRAN, but the baseline tool for integrated modeling and the bulk of the component

models are with TD. Since the MSFC heritage for thermal modeling of ablation has been with the in-house ABL code and the ablation capability in TD is a relatively new addition, a validation process was undertaken to benchmark the TD ABLATE subroutine for use on Ares-I. This resulted in the development of a new subroutine by Cullimore & Ring Technologies, Inc. called ABLATERATE.

### PHYSICS OF ABLATION:

The process of physical ablation occurs during extreme convective heating environments, such as that experienced for a re-entry vehicle, such as the Space Shuttle Orbiter.

Ablation materials undergo chemical decomposition, or pyrolysis, which forms a char layer as shown in Figure 2. During this process, energy is transferred away by the pyrolysis gasses and the surface of the

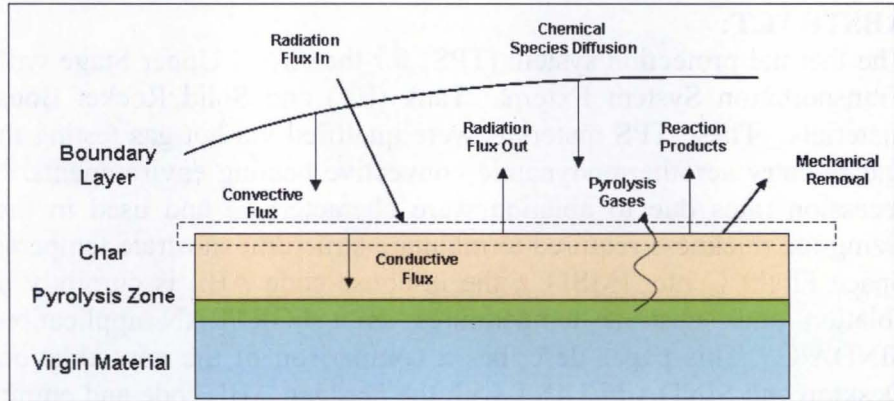


Figure 2: Surface Ablation Characteristics

material recedes with time. In addition, the heating region consists of highly ionized air that has dissociated, resulting in complex chemical reactions at the surface and within the boundary layer. The energy balance between the convective energy (sensible), chemical energy and net radiation at the TPS surface is as follows<sup>1</sup>:

$$\underbrace{\rho_e u_e C_H (H_r - h_{e_w})}_{\text{Sensible Energy Rate}} + \underbrace{\rho_e u_e C_M \left[ \sum (Z_{i_e}^n - Z_{i_w}^n) h_i^{T_w} - B' h_w \right] + \dot{m}_c h_c + \dot{m}_g h_g}_{\text{Chemical Energy Rate}} + \underbrace{\alpha_w q_{rad} - F \sigma \epsilon_w T_w^4 - q_{cond}}_{\text{Net Radiation Energy Rate}} = 0$$

Internally within the TPS material, the energy balance includes the effects of the surface recession and pyrolysis gas as follows:

$$\underbrace{\rho c_p \frac{\partial T}{\partial t}}_{\text{Energy Storage}} = \underbrace{\frac{1}{A} \frac{\partial}{\partial x} \left( kA \frac{\partial T}{\partial x} \right)}_{\text{Conduction Rate}} + \underbrace{(h_g - \bar{h}) \frac{\partial \rho}{\partial t}}_{\text{Pyrolysis Energy}} + \underbrace{\dot{s} \rho c_p \frac{\partial T}{\partial x}}_{\text{Recession Rate}} + \underbrace{\frac{\dot{m}}{A} \frac{\partial h_g}{\partial x}}_{\text{Pyrolysis Gas Convection}}$$


Without pyrolysis & ablation, the sensible gaseous convective heat transfer and enthalpy calculations including real gas effects can be simplified to the form typically provided by the thermal analyst by aerothermodynamic environments codes. This surface energy balance simplifies to:

$$\underbrace{h_c (H_r - H_w)}_{\text{Gaseous Convection}} + \underbrace{\alpha_w q_{rad} - F \sigma \epsilon_w T_w^4}_{\text{Surface Net Radiation}} - q_{cond} = 0$$

Internally to the TPS material, the recession of the material thickness affects the conduction and thermal capacitance of the remaining material. This energy balance can

be shown by the following equation (where  $s$  represents the amount of recession from the original TPS surface as shown in the Figure below):

$$\rho_p \frac{\partial T}{\partial t} = \frac{1}{A} \frac{\partial}{\partial x} \left( kA \frac{\partial T}{\partial x} \right) + \dot{s} \rho_p \frac{\partial T}{\partial x}$$

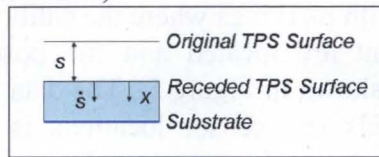

These last two equations more appropriately represent the governing equations inherent to the MSFC ABL and TD ABLATE modeling approaches. The complex chemical energy balance is not explicitly modeled, so an examination of the method of acquiring the TPS ablation properties empirically is discussed in the next section to illustrate how this element of the physics is addressed.

### ET/SRB TPS ABLATION TESTING METHODOLOGY:

The TPS material qualification for the Space Transportation System ET and SRB programs for the ascent and plume heating environments was accomplished using various arc-jet and hot gas wind tunnel facilities.



Figure 3: MSFC Hot Gas Facility

To illustrate the process used to characterize the TPS materials, the Marshall Convergent Coating (MCC-1) will be used as an example<sup>2</sup>. The MCC-1 is a MSFC developed TPS material formulated to replace the Marshall Sprayable Ablator-2 (MSA-2) on the SRB forward assembly, systems tunnel covers and aft skirt. The MCC-1 uses convergent spray technology and consists of 8% hollow spherical glass, 9% cork, and 83% two-part epoxy by weight. The qualification testing of the material was performed at MSFC's Improved Hot Gas Facility, which is a Mach 4 convective heating wind tunnel capable of 3.5 to 25 Btu/hr/ft<sup>2</sup>-s heat flux and an optional 300kW radiant heat system capable of a 0 to 35 Btu/hr/ft<sup>2</sup>-s heat flux.

The angle of incidence between a test panel and the flow can be varied to achieve various heating conditions. An aluminum calibration panel (12x19-inch) including 20 Medtherm Schmidt-Boelter type heat flux gages, pressure measurements, and backside temperature measurements was used to determine the hot wall gaseous heating rates (see Figure 4). This heating rate was then "normalized" to a cold wall heating rate using this equation:

where:

$$\dot{q}_{cw} = \dot{q}_{hw} \left[ \frac{(T_r - T_{cw})}{(T_r - T_w)} \right]$$

$\dot{q}_{cw}$  = Cold wall heat rate (Btu/ft<sup>2</sup>/s)  
 $\dot{q}_{hw}$  = Hot wall heat rate (Btu/ft<sup>2</sup>/s)  
 $T_r$  = Adiabatic wall recovery temp (°F)  
 $T_{cw}$  = Cold wall reference temp (0°F)  
 $T_w$  = Calibration Plate Surface temp (°F)  
 $r^{**}$  = Corrected recovery factor  
 $T_r = r^{**} \times T_{total}$

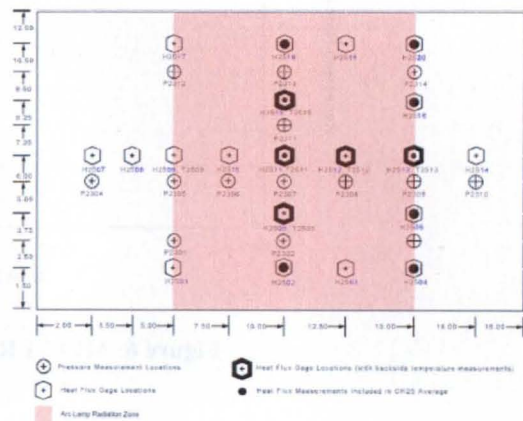


Figure 4: Calibration Test Panel

After testing of TPS panel, the char layer is removed from tested panel and detailed micrometer measurements are used to determine recession rate down to the virgin TPS. A pre-test panel with markings where the calibration panel measurement are located and the post-test charred panel are shown in Figure 5. The data from multiple test panels and sensor locations is then used to perform a linear least squares curve fit as follows:

$$\dot{r} = k\dot{q}_{cw}^x$$

- where:
- $\dot{q}_{cw}$  = Cold wall heat rate (Btu/ft<sup>2</sup>/s)
  - $k$  = Least squares fit y-intercept
  - $\dot{r}$  = Recession rate (mils/sec)
  - $x$  = Least squares fit slope

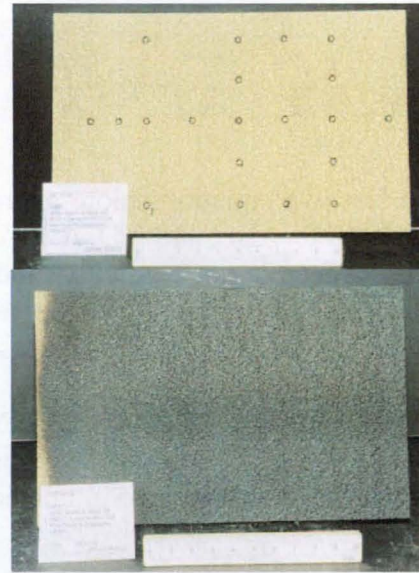


Figure 5: Pre- and Post-Test Panel

The MCC-1 curve fits, including the 95 percentile upper limit, which is calculated for use as the design recession curve fit are shown in Figure 6. Since the test environment includes the flight-like flow boundary conditions and the TPS undergoes the pyrolysis and char layer formation, the affects of the chemical reactions and mechanical erosion are inherently included in the empirical recession data. By removing the char layer prior to the thickness measurements, the recession to the char-to-virgin material interface is represented in the data. Since the ablation temperature is determined from Thermogravimetric Analysis (TGA) testing of the TPS material, the value represents the onset of pyrolysis and charring, which is appropriate for the char-to-virgin material interface typically set as the boundary temperature in thermal analysis codes.

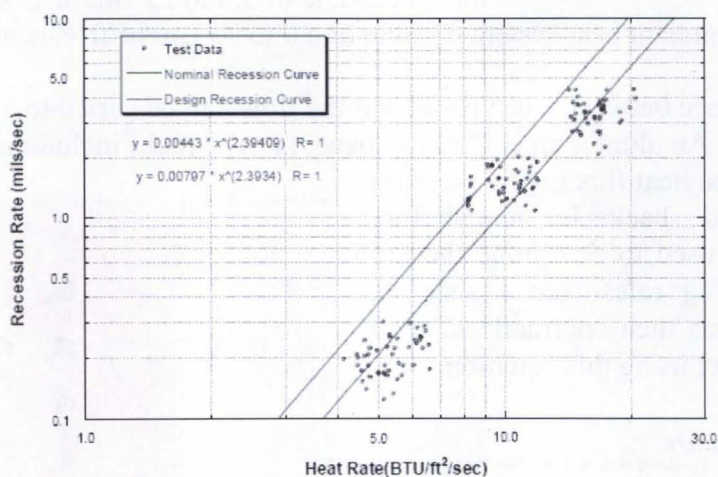


Figure 6: MCC-1 Recession Versus Heat Rate

## THERMAL DESKTOP ABLATE SUBROUTINE:

The TD with SINDA/FLUINT software code includes the ABLATE subroutine to simulate 1-dimensional surface ablation and the material recession. The input parameters for this routine are heat of ablation ( $Q_{abl}$ ) and the ablation temperature of the TPS. Once ablation temperature is reached, the surface node is held constant by the BDYNOD utility. Then, the surface node is “shrunk” to simulate the mass loss due to ablation, which involves altering the nodal capacitance and linear conductor to the adjacent node within the thickness of the TPS. Instead of reducing the node size to very small thicknesses, which can result in small a capacitance over sum of conductors (CSG) ratio and small numerical timesteps, the node is “collapsed” once the mass drops below 50% of its original value (based on RTMIN default). The capacitance and energy from the “collapsed” node is then reassigned to the “next” node and changed to an arithmetic node which still participates in the network. This allows the model

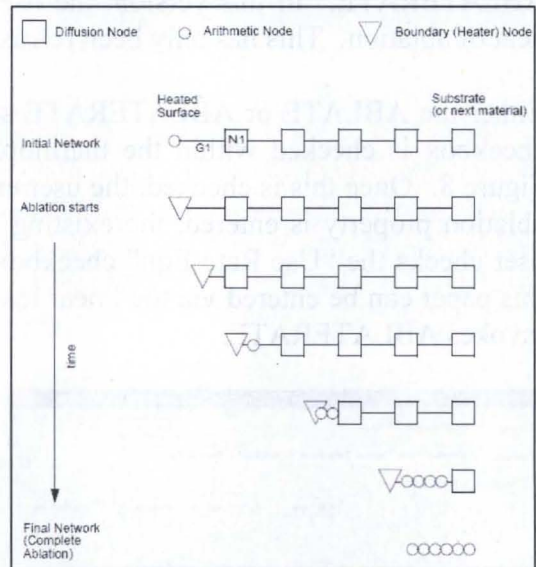


Figure 7: TD Ablation Nodal Network

nodalization to remain unchanged and not affect surface heating logic. This process continues through the nodes representing the thickness of the material as long as the heating is sufficient to keep the surface at the ablation temperature. This process is illustrated graphically in Figure 7<sup>3</sup>. The user defines the number of nodes and an array of initial thicknesses. The final node can be designated such that it is not allowed to completely ablate, which would simulate a burn through scenario.

For the Ares-I TPS materials, the heat of ablation is not explicitly defined, but rather the recession rate normalized the cold wall heat flux is defined as outlined previously. An attempt was made to generate an effective heat of ablation using the recession data via the following equation:

$$Q_{abl} = \frac{12000 \times \dot{q}_{net}''}{\dot{r} \times \rho_{TPS}}$$

where:

- $\dot{r}$  = recession rate (mils/sec)
- $\dot{q}_{net}''$  = Net surface cold wall heat flux (Btu/sec/ft<sup>2</sup>)
- $\rho_{TPS}$  = TPS density (lbm/ft<sup>3</sup>)
- $Q_{abl}$  = Heat of Ablation (Btu/lbm)

This approach proved laborious and difficult to implement. Sensitivity studies were required to ensure the proper energy balance was being maintained and that the model was converging properly. Comparisons of results with MSFC's ABL code revealed inconsistencies in the accuracy of this approach, so Cullimore & Ring Technologies, Inc.

(C&R) was consulted on these issues. Additionally, a request for a simplified method to enter the hot wall convective heating enthalpy and convection coefficient to be interpolated as a function of hot wall temperature was made.

**THERMAL DESKTOP ABLATERATE SUBROUTINE:**

The C&R response was the development of the alternate ablation subroutine, ABLATERATE. In this version, the user defines the linear recession curve instead of heat of ablation. This has only been released as a Beta test version at this point.

Either the ABLATE or ABLATERATE subroutine is invoked when the “Use Ablation” checkbox is checked within the thermophysical property definition panel as shown in Figure 8. Once this is checked, the user enters the ablation temperature and if the heat of ablation property is entered, the existing ABLATE routine is utilized. However, if the user checks the “Use Rate Eqn” checkbox, then the recession rate equation discussed in this paper can be entered via the linear least squares intercept and slope (Figure 9), which invokes ABLATERATE.

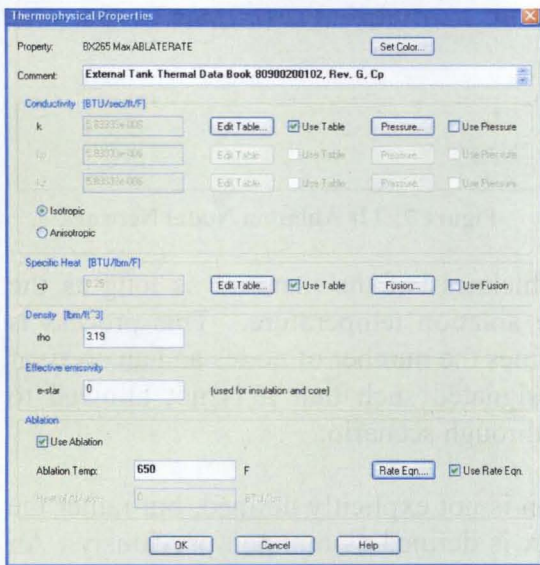


Figure 8: Entering Ablation Properties

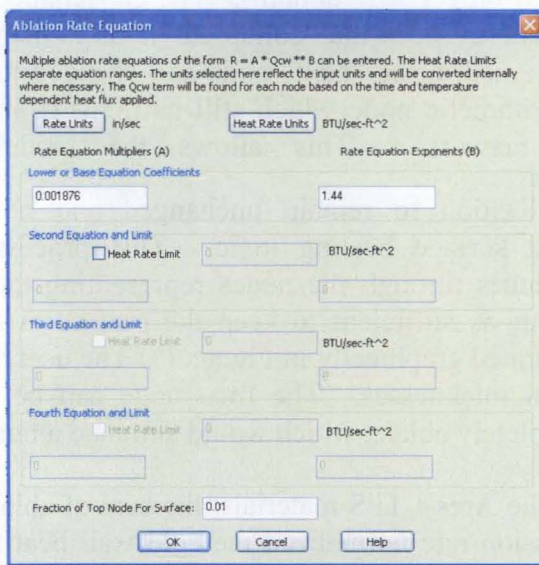
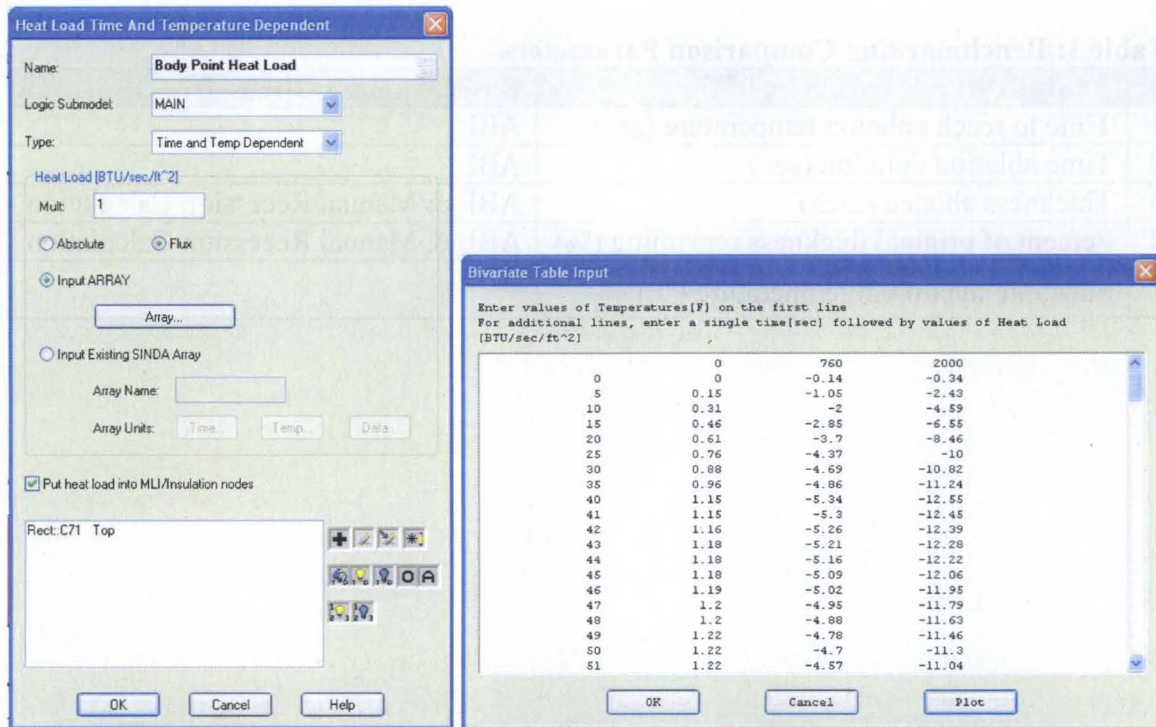


Figure 9: Entering Recession Rate Equation

Another parameter added for the user is the “Fraction of Top Node for Surface”, which defaults to 0.01 as shown at the bottom of Figure 9. This parameter allows the user to assign a finite capacity to the surface node, which assists in the numerical stability for very high heating rate problems. It is recommended that the user perform a sensitivity study of this parameter to ensure optimum run-time with accurate results. The user can also alter the nodal thicknesses representing the TPS below the surface node.

Another change to Thermal Desktop implemented to improve the ease of entering aero-thermal heating rates is the ability to enter a heat load that is a function of both time and temperature. If the user adds this type of heat load, an input bivariate array can be defined with the temperatures for which aero-thermal data is available and the

corresponding heat load versus time at each of these temperatures. Example panels demonstrating this feature are shown in Figure 10.



**Figure 10: Alternate Method of Entering Bi-Variate Aero-Thermal Heat Loads**

### COMPARISON TO MSFC HERITAGE ABL CODE:

A parametric study of cases has been performed to compare the new C&R ABLATERATE subroutine to the empirical recession rate data as well as to the results from the MSFC heritage code ABL. The ultimate indicator of accuracy for these model results is whether the material recession calculations match the test data, since this is the real grounding aspect of this approach. The primary purpose of benchmark comparisons to the MSFC ABL code is to verify that through thickness temperatures and substrate temperature predictions are comparable using the “collapsing” nodal network approach.

In order to bracket the TPS cases anticipated for Ares I Upper Stage design, a range of TPS materials and associated ablation temperatures, recession rates, and thermo-physical properties were assessed. Also, a range of material thicknesses and convective heating rates were simulated in ABLATERATE and ABL for comparison. The thicknesses were varied to simulate cases where the substrate is only slightly heated to cases where the TPS is completely ablated. The cases were initialized to 80°F at TIME=0.0 and utilized typical heating profiles for the current Ares I aerothermodynamic heating environment with scaling as necessary to achieve the desired test case. Table 1 details the parameters that were compared.

**Table 1: Benchmarking Comparison Parameters**

#	Analysis Result Parameter	Basis of Comparison
1	Time to reach ablation temperature (sec)	ABL
2	Time ablation duration (sec)	ABL
3	Thickness ablated (inch)	ABL & Manual Recession Calculation
4	Percent of original thickness remaining (%)	ABL & Manual Recession Calculation
5	Substrate maximum temperature (°F)	ABL



**Table 2: Thermal Desktop Benchmark Results**

Case	Material	Original Thickness (in)	Peak $q_{cw}$ (Btu/ft <sup>2</sup> -s)	Analysis Benchmark Parameter Difference						
				1 (% Difference)	2 (% Difference)	3 (% Difference)		4 (% Difference)		5 (Temperature Difference)
						vs. ABL	vs. Manual	vs. ABL	vs. Manual	
1	BX-265	0.50	8.41	1.1%	0.7%	+2.4%	-1.3%	4.7%	-1.3%	1.4°F
2										

EXAMPLE – RESULTS NOT FILLED IN

## **SUMMARY & CONCLUSIONS:**

Based on the implementation of the empirical TPS recession test data and the comparison to the heritage MSFC ABL code, the use of Thermal Desktop's new ABLATERATE routine for in-house Ares-I Upper Stage ascent convective aero-thermal heating of TPS is valid.

Due to EPA regulations, some of the heritage ET/SRB materials are being reformulated for Ares I and will undergo re-qualification testing. Additional validation of the predictions will be done as part of this testing.

Future analytical studies of plume impingements areas from solid rocket motor firings or hydrazine thrusters will be performed to determine the viability of the ABLATERATE approach for these very high heat flux, but short duration events. More important than the operation of Thermal Desktop numerically for these environments is the derivation of the proper empirical data to represent the material performance under these unique loading environments.

Additionally, comparisons of ABLATERATE results to the Aerotherm Charring Material Thermal Response and Ablations Program (CMA) code are planned for materials with sufficient property data available.

## **ACKNOWLEDGEMENTS:**

The authors would like to acknowledge the assistance of Mr. Darrell Davis of MSFC for his insight into the TPS testing processes. The authors would also like to acknowledge Mr. Mark Hooton and Mr. Maurice Prendergast of MSFC for their generating the results data from ABL for the Thermal Desktop comparisons. The authors would like to thank Mr. David Johnson & Mark Welch of Cullimore & Ring, Inc. for generating the ABLATERATE capability in response to our request.

## **References:**

1. User's Guide, Non-Proprietary Aerotherm Charring Material Thermal Response and Ablation Program, CMA87S, November 1987.
2. AIAA-2002-3334, "Recession Curve Generation for Space Shuttle Solid Rocket Booster Thermal Protection System Coatings", Kanner, Stuckey & Davis. June 2002.
3. User's Manual, SINDA/FLUINT General Purpose Thermal/Fluid Network Analyzer, Version 5.0. C&R Technologies. Oct. 2006.

# Thermal & Fluids Analysis Workshop



## ABLATION MODELING OF ARES-I UPPER STAGE THERMAL PROTECTION SYSTEM USING THERMAL DESKTOP

Sept. 13, 2007


*Authors:*

*John Sharp*

*Tim Page*

*National Aeronautics & Space Administration*


*George C. Marshall Space Flight Center*

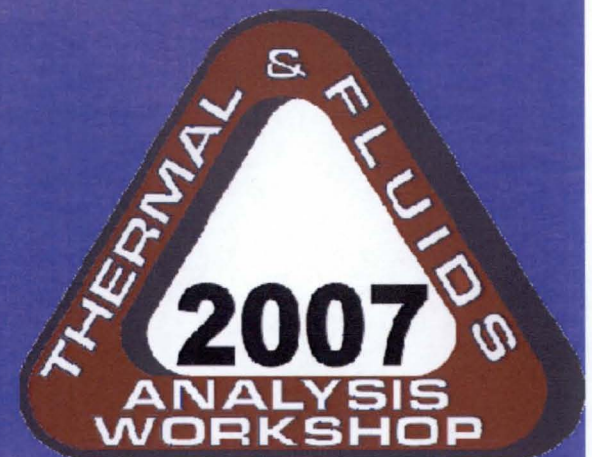



# Topics


---




- ◆ **Ares I Upper Stage Description**
- ◆ **Physics of TPS Ablation**
- ◆ **STS SRB/ET TPS Ablation Testing**
- ◆ **Thermal Desktop ABLATE subroutine**
- ◆ **New ABLATERATE subroutine**
- ◆ **Comparison to MSFC Heritage ABL Code**
- ◆ **Summary & Conclusions**
- ◆ **Acknowledgements & References**

## Ares Upper Stage Description

- ◆ Ares I Upper Stage consists of Liquid Hydrogen & Liquid Hydrogen tanks to fuel the J-2X engine. Various protuberances (RCS, feedlines, etc.)
- ◆ The cryogenic tank insulations and protuberance aeroheating insulations are Shuttle-derived materials, primarily from External Tank.
  - ◆ Spray-On Foam Insulation (SOFI) – polyurethane-type closed cell foam
  - ◆ Super Lightweight Ablator (SLA)

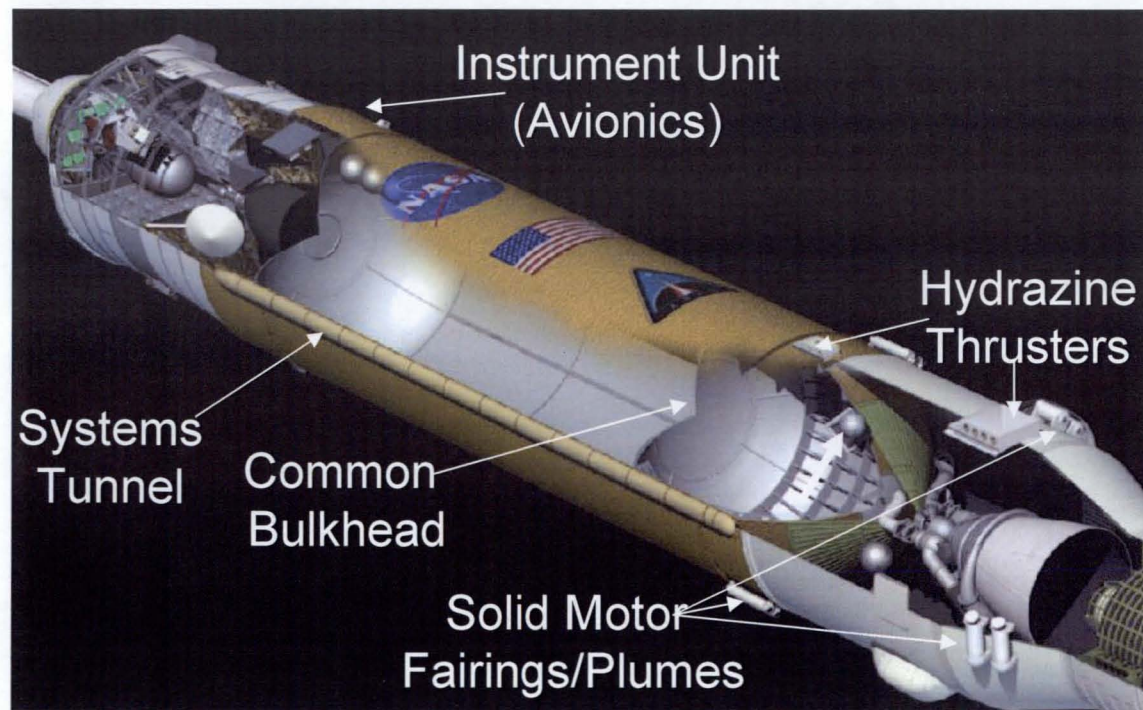

**Ares-I Upper Stage**

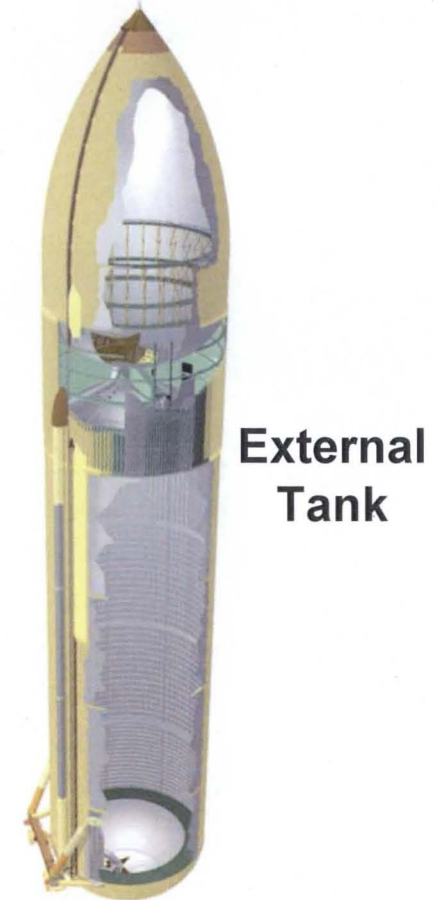


- ◆ Surface energy balance (convective heating & thermo-chemical erosion):

$$\underbrace{\rho_e u_e C_H (H_r - h_{e_w})}_{\text{Sensible Energy Rate}} + \underbrace{\rho_e u_e C_M \left[ \sum (Z_{i_e}^n - Z_{i_w}^n) h_i^{T_w} - B' h_w \right] + \dot{m}_c h_c + \dot{m}_g h_g}_{\text{Chemical Energy Rate}} + \underbrace{\alpha_w q_{rad} - F \sigma \epsilon_w T_w^4 - q_{cond}}_{\text{Net Radiation Energy Rate}} = 0$$

- ◆ Internal energy balance (for recessing surface):

$$\underbrace{\rho c_p \frac{\partial T}{\partial t}}_{\text{Energy Storage Rate}} = \underbrace{\frac{1}{A} \frac{\partial}{\partial x} \left( kA \frac{\partial T}{\partial x} \right)}_{\text{Conduction Rate}} + \underbrace{(h_g - \bar{h}) \frac{\partial \rho}{\partial t}}_{\text{Pyrolysis Energy Rate}} + \underbrace{\dot{s} \rho c_p \frac{\partial T}{\partial x}}_{\text{Recession Rate}} + \underbrace{\frac{\dot{m}}{A} \frac{\partial h_g}{\partial x}}_{\text{Pyrolysis Gas Convection Rate}}$$

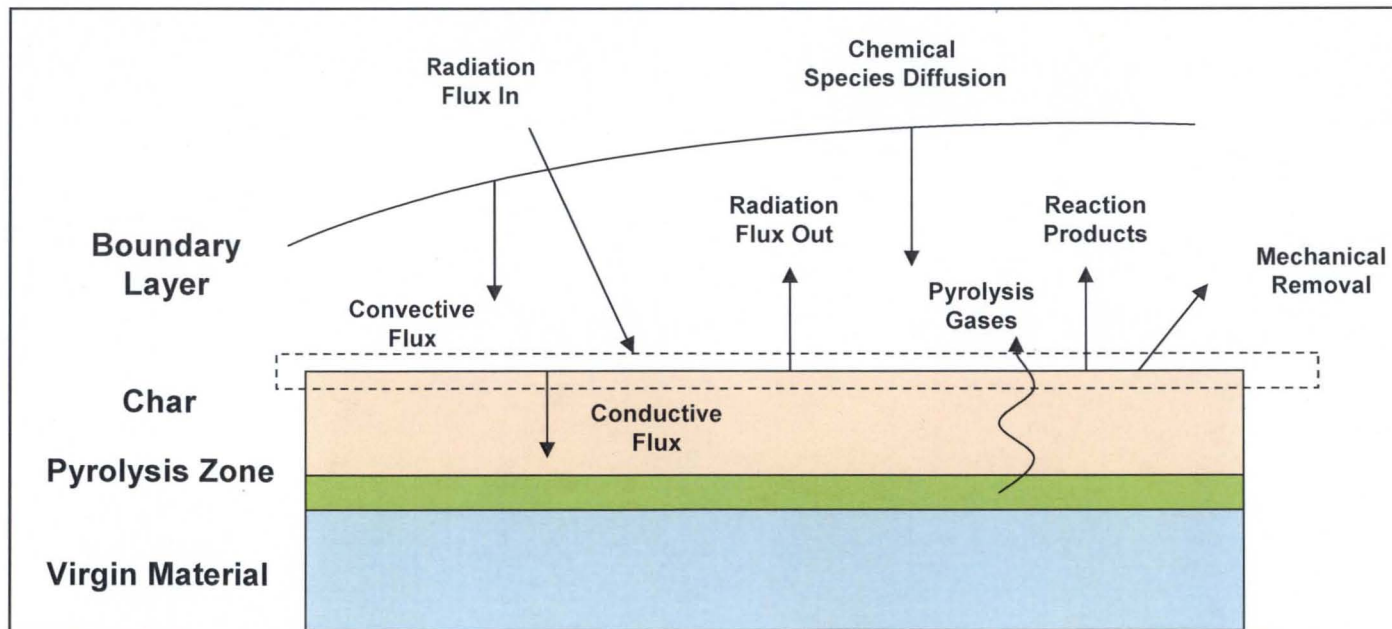


- ◆ Without pyrolysis & ablation, surface energy balance simplifies to:

$$\underbrace{h_c(H_r - H_w)}_{\text{Gaseous Convection}} + \underbrace{\alpha_w q_{rad} - F\sigma\epsilon_w T_w^4 - q_{cond}}_{\text{Surface Net Radiation}} = 0$$

- ◆ Internal energy balance (for recessing surface without pyrolysis):

$$\rho c_p \frac{\partial T}{\partial t} = \frac{1}{A} \frac{\partial}{\partial x} \left( kA \frac{\partial T}{\partial x} \right) + \dot{s} \rho c_p \frac{\partial T}{\partial x}$$

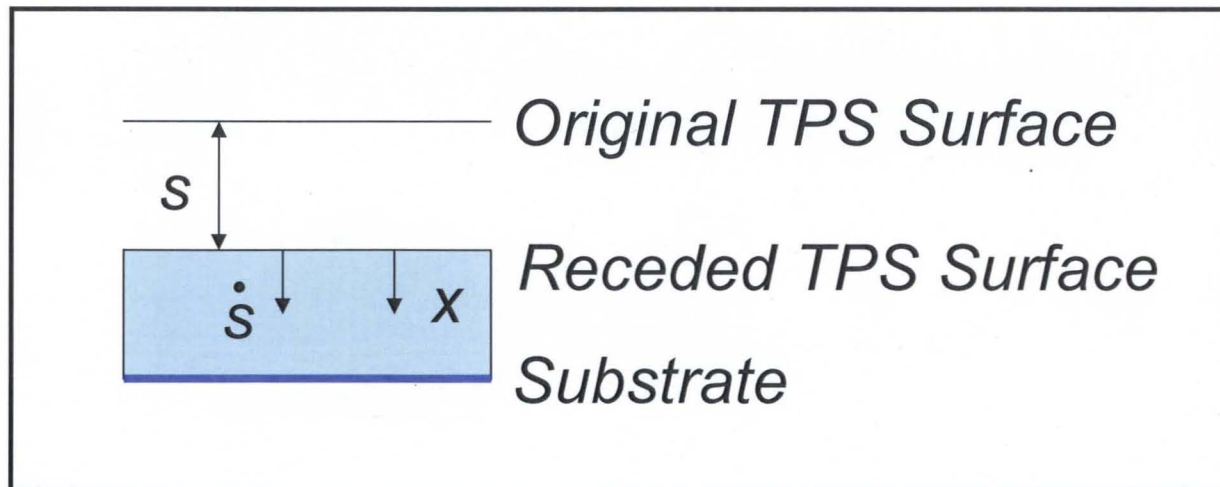

- ◆ For the SRB and ET TPS materials, arc-jet and hot gas test facilities have been used to characterize the original & replacement materials.
- ◆ An example replacement material is the Marshall Convergent Coating (MCC-1) tested in MSFC's Improved Hot Gas Facility (IHGF)
  - ◆ Mach 4 convective heating wind tunnel capable of 3.5 to 25 Btu/ft<sup>2</sup>-s
  - ◆ 300 kW radiant heat system capable of 0 to 35 Btu/ft<sup>2</sup>-s
- ◆ MCC-1 uses convergent spray technology
- ◆ Consists of 8% hollow spherical glass, 9% cork, and 83% two-part epoxy by weight
- ◆ Replaced Marshall Sprayable Ablator-2 (MSA-2) on SRB forward assembly, systems tunnel covers, and aft skirt.





- ◆ Calibration panels are used to determine hot wall heating rates for a given panel size and “wedge” angle. Data is then “normalized” to 0°F (460R) cold wall heat rate by:

$$\dot{q}_{cw} = \dot{q}_{hw} \left[ \frac{(T_r - T_{cw})}{(T_r - T_w)} \right]$$

where:

$\dot{q}_{cw}$  = Cold wall heat rate (Btu/ft<sup>2</sup>/s)

$\dot{q}_{hw}$  = Hot wall heat rate (Btu/ft<sup>2</sup>/s)



$T_r$  = Adiabatic wall recovery temp (°F)

$$T_r = r^* \times T_{total}$$


$T_{cw}$  = Cold wall reference temp (0°F)

$T_w$  = Calibration Plate Surface temp (°F)

$r^*$  = Corrected recovery factor

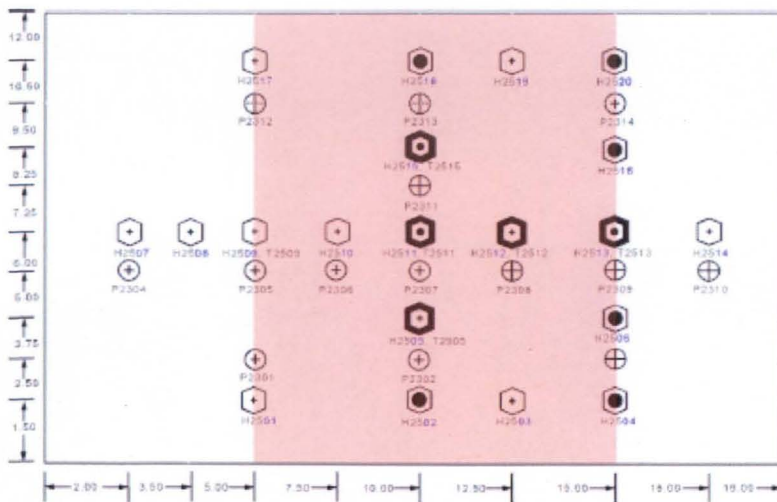

Calibration Panel

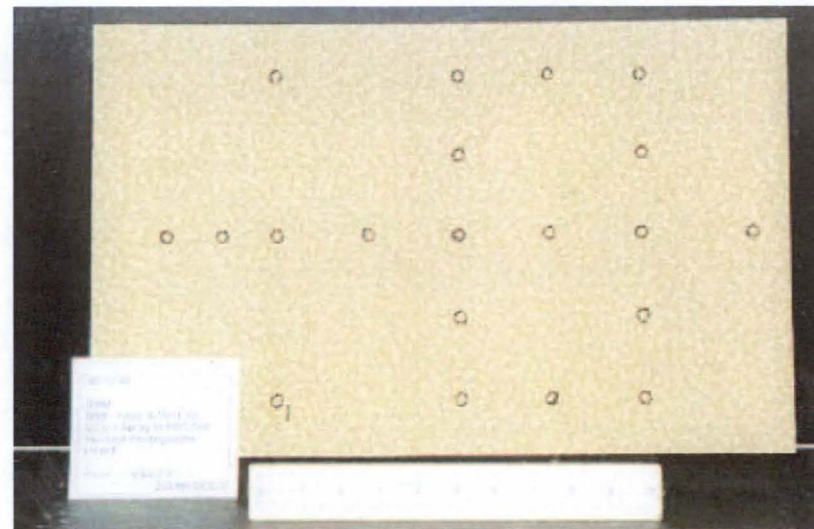

MCC-1 Test Panel

- ◆ Char layer is removed from tested panel and micrometer measurements are used to determine recession rate. A linear least-squares curve fit is generated. A 95% upper limit is calculated for use as the design recession curve.


$$\dot{r} = k\dot{q}_{cw}^x$$

where:  $\dot{q}_{cw}$  = Cold wall heat rate (Btu/ft<sup>2</sup>/s)


$k$  = Least squares fit y-intercept

$\dot{r}$  = Recession rate (mils/sec)

$x$  = Least squares fit slope

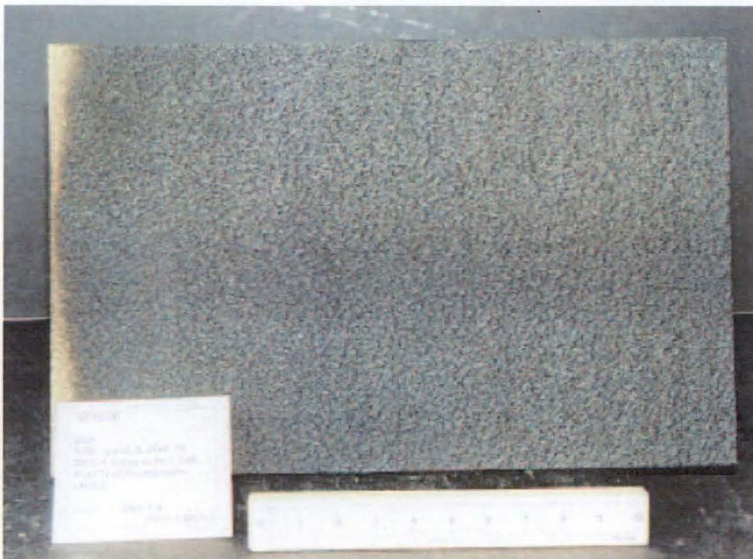

Post-test panel

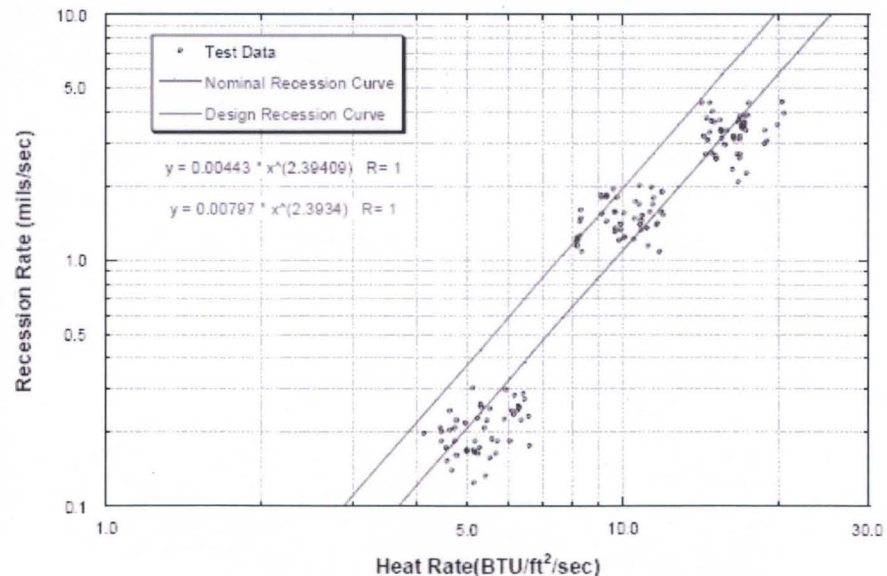

MCC-1 Recession Curve



- ◆ For Ares I Upper Stage (ET/SRB derived materials), the material recession rate and ablation temperature are available, but not heat of ablation.
- ◆ Calculating an effective Heat of Ablation,  $Q_{abl}$ , using equations below gave varying levels of success.
- ◆ This approach proves difficult to implement, and required sensitivity studies to ensure proper energy balance was being maintained.
- ◆ Comparisons to MSFC's ABL code were performed.

$$Q_{abl} = \frac{12000 \times \dot{q}_{net}''}{\dot{r} \times \rho_{TPS}}$$

where:

- $\dot{r}$  = recession rate (mils/sec)
- $\dot{q}_{net}''$  = Net surface cold wall heat flux (Btu/sec/ft<sup>2</sup>)
- $\rho_{TPS}$  = TPS density (lbm/ft<sup>3</sup>)
- $Q_{abl}$  = Heat of Ablation (Btu/lbm)

- ◆ Cullimore & Ring, Inc. was consulted on the issues with ABLATE as well as a request for a method to simplify convective heating enthalpy & convection coefficient versus hot wall temperature.
- ◆ C&R generated the ABLATERATE subroutine, which is undergoing “Beta” testing.
- ◆ User chooses “Use Ablate” for thermophysical property. Then, “Rate Eqn” coefficients can be entered as shown below:

Thermophysical Properties

Property: Bx265 Max ABLATERATE

Comment: External Tank Thermal Data Book 80900200102, Rev. G, Cp

Conductivity [BTU/sec/ft/F]

k: 5.83333e-006 [Edit Table]  Use Table [Pressure...]  Use Pressure

ky: 5.83333e-006 [Edit Table]  Use Table [Pressure...]  Use Pressure

kz: 5.83333e-006 [Edit Table]  Use Table [Pressure...]  Use Pressure

Isotropic  Anisotropic

Specific Heat [BTU/lbm/F]

cp: 0.25 [Edit Table]  Use Table [Fusion...]  Use Fusion

Density [lbm/ft^3]

rho: 3.19

Effective emissivity

e-star: 0 (used for insulation and core)

Ablation

Use Ablation

Ablation Temp: 6500 F [Rate Eqn...]  Use Rate Eqn

OK Cancel Help

Ablation Rate Equation

Multiple ablation rate equations of the form  $R = A * Q_{cw} ** B$  can be entered. The Heat Rate Limits separate equation ranges. The units selected here reflect the input units and will be converted internally where necessary. The  $Q_{cw}$  term will be found for each node based on the time and temperature dependent heat flux applied.

Rate Units: in/sec Heat Rate Units: BTU/sec-ft^2

Rate Equation Multipliers (A) Rate Equation Exponents (B)

Lower or Base Equation Coefficients

0.001876 1.44

Second Equation and Limit

Heat Rate Limit: 0 BTU/sec-ft^2

0 0

Third Equation and Limit

Heat Rate Limit: 0 BTU/sec-ft^2

0 0

Fourth Equation and Limit

Heat Rate Limit: 0 BTU/sec-ft^2



0 0

Fraction of Top Node For Surface: 0.01

OK Cancel Help

Fraction of Top Node for Surface

- ◆ Bi-Variate Interpolation of Heating Rates as function of Hot Wall Temperature and Time.
- ◆ After entering Thermal Desktop “Heat Load”, a bivariate array of available Temperatures (to be interpolated between) and the corresponding heat flux versus time can be entered.

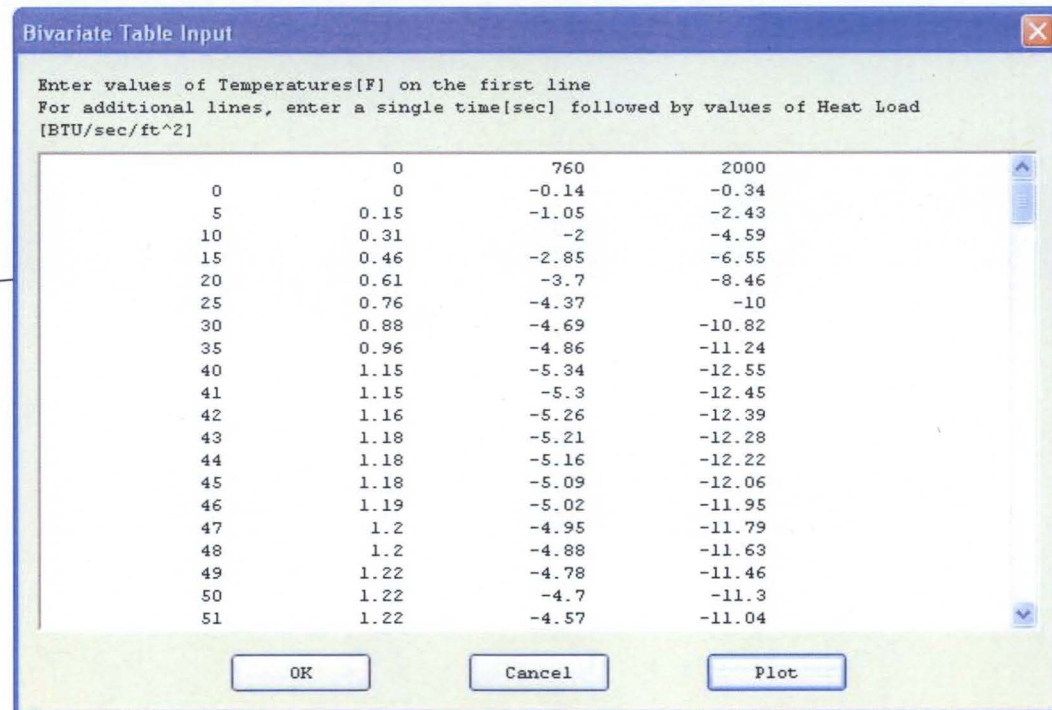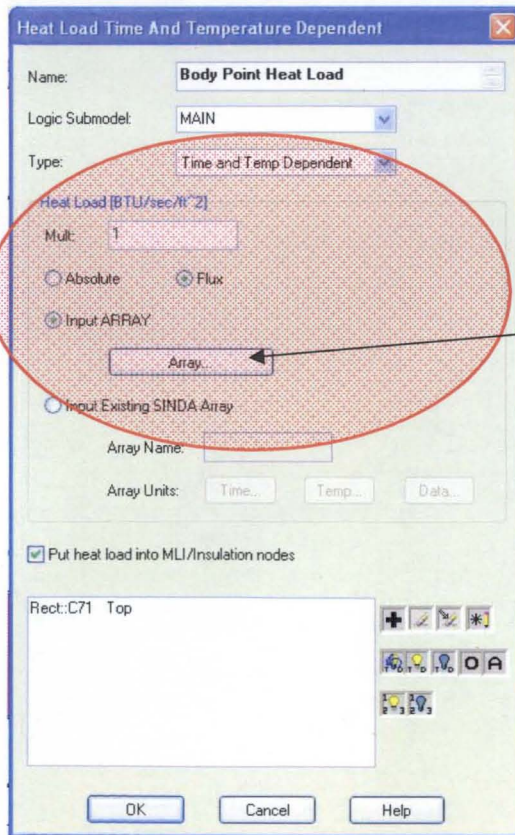

- MSFC has conducted a comprehensive parametric study comparing ABLATERATE to the in-house ABL code. A range of materials, thicknesses, heating rates were used to exercise the tools.

				Analysis Benchmark Parameter Difference						
Case	Material	Original Thickness (in)	Peak $q_{cw}$ (Btu/ft <sup>2</sup> -s)	1 (% Difference)	2 (% Difference)	3 (% Difference)		4 (% Difference)		5 (Temperature Difference)
						vs. ABL	vs. Manual	vs. ABL	vs. Manual	
1	BX-265	0.50	8.41	1.1%	0.7%	+2.4%	-1.3%	4.7%	-1.3%	1.4°F
2										

**EXAMPLE - RESULTS NOT FILLED IN**



## Summary & Conclusions

---



- ◆ Based on the comparison to MSFC's ABL tool & empirical test data, the use of ABLATERATE for in-house Ares I Upper Stage ascent convective aero-thermal heating ablation is valid.
- ◆ Due to EPA regulations, many of the heritage ET/SRB materials are being reformulated for Ares I and will undergo re-qualification testing. Additional validation of the predictions will be done as part of this.
- ◆ Future work for high flux areas (such as solid motor plume impingements) will be performed to determine viability of ABLATERATE approach for very high, but short heating events. Contingent on testing and empirical data.
- ◆ Future comparisons are planned using the Aerotherm Charring Material Thermal Response and Ablations Program (CMA).





## Acknowledgements & References

---



- ◆ The authors would like to acknowledge the assistance of Mr. Darrell Davis of MSFC for his insight into the TPS testing processes.
- ◆ The authors would like to acknowledge Mr. Mark Hooton and Mr. Maurice Prendergast of MSFC for their ABL comparisons.
- ◆ The authors would like to thank Mr. David Johnson & Mark Welch of Cullimore & Ring, Inc. for generating the ABLATERATE capability.

### References:

1. User's Guide, Non-Proprietary Aerotherm Charring Material Thermal Response and Ablation Program, CMA87S, November 1987.
2. AIAA-2002-3334, "Recession Curve Generation for Space Shuttle Solid Rocket Booster Thermal Protection System Coatings", Kanner, Stuckey & Davis. June 2002.
3. User's Manual, SINDA/FLUINT General Purpose Thermal/Fluid Network Analyzer, Version 5.0. C&R Technologies. Oct. 2006.