

LASER RADAR STUDY USING RESONANCE ABSORPTION
FOR REMOTE DETECTION OF AIR POLLUTANTS

Takashi Igarashi

Radio Research Laboratories, Ministry of Posts
and Telecommunications, Koganei, Tokyo, Japan

ABSTRACT

A laser radar using resonance absorption has an advantage of increased detection range and sensitivity compared with that achieved by Raman or resonance back scattering .

In this paper, new laser radar system using resonance absorption is proposed and results obtained from this laser radar system are discussed.

NO_2 , SO_2 gas has an absorption spectrum at 4500 \AA and 3000 \AA respectively as shown in Fig. 1. A laser light including at least a set of an absorption peak λ_1 and a valley λ_2 is emitted into a pollutant atmosphere. The light reflected with a topographical reflector or an atmospheric Mie scattering as distributed reflectors is received and divided into two wavelength components λ_1 , λ_2 . From the ratio of these two components $Y(x)$, the distribution of the pollutant gas $n(x)$ can be calculated by

$$n(x) = \frac{1}{2(\sigma_1 - \sigma_2)} \frac{dY(x)}{dx}$$

, where σ_1 , σ_2 correspond to the absorption cross sections of the pollutant gas at λ_1 and λ_2 respectively.

The laser radar system used in the investigation is shown in Fig. 2 and consists of a dye laser transmitter, an optical receiver with a special monochrometer and a digital processor. Table 1 shows the molecular constants of NO_2 , and SO_2 and the dye laser used in this experiment.

		NO ₂	SO ₂
λ_1	(\AA)	4482	3001
λ_2		4469	3014
$\sigma_1 - \sigma_2$ (cm ²)		2.0×10^{-19}	2.5×10^{-18}
$\lambda_1 - \lambda_2$ (\AA)		13	13
Dye Material		calcein blue	SHGed Rhodamine B
Spectrum width (\AA)		30	30
Pumping Source		Sum of SHGed and fundamental Nd: YAG	SHGed Nd: YAG

Table 1 Molecular constants of NO₂ and SO₂ and dye laser used

In this system, the absolute concentration of the pollutant gas can be measured in comparison with a standard gas cell. The concentration of NO₂, SO₂ as low as 0.1 ppm have been measured at 100 m depth resolution. For a 1 mJ laser output, the observable range of this system achieved up to 300 m using the distributed Mie reflector.

The capability and technical limitation of the system will be discussed in detail.

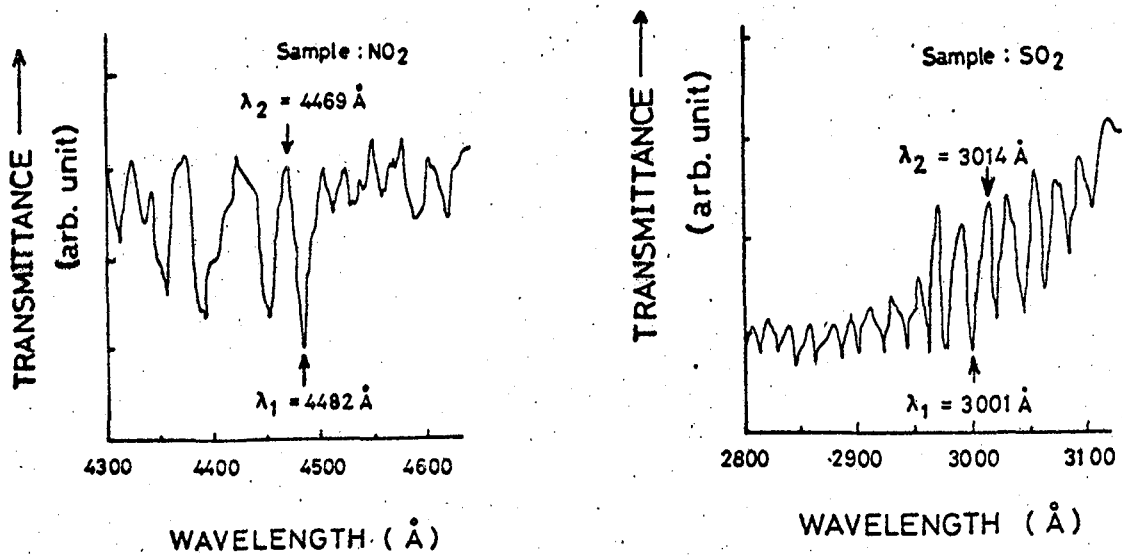


Fig.1 Absorption spectrum of NO₂ and SO₂

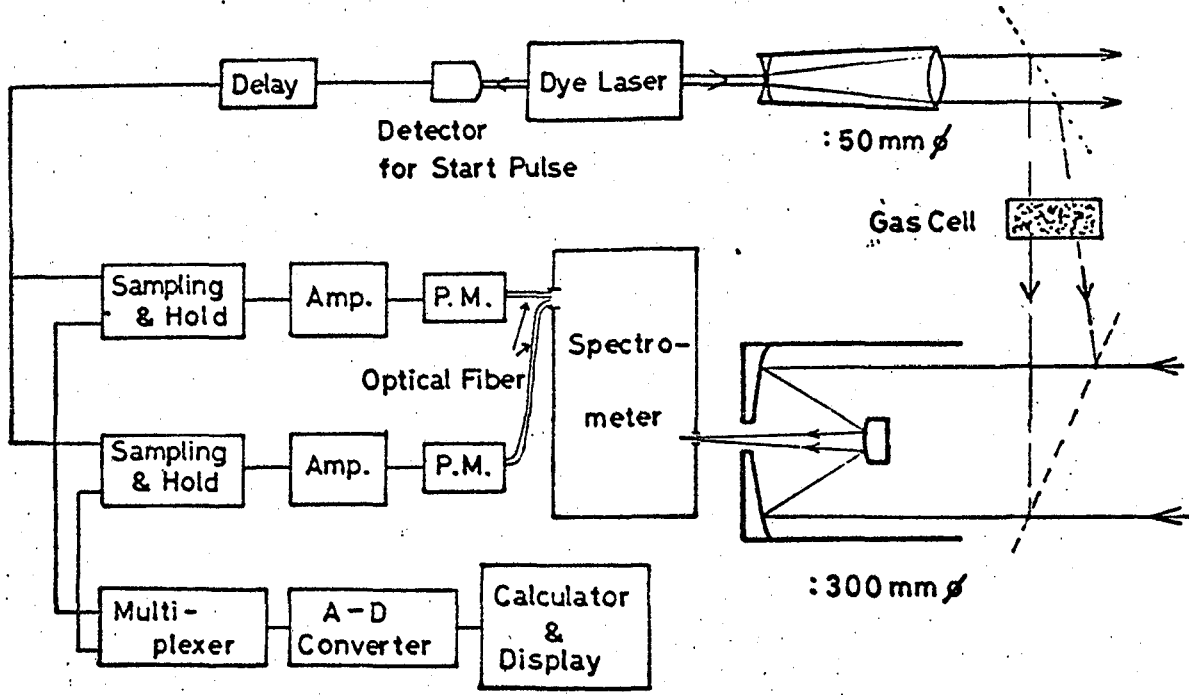


Fig.2 Schematic diagram of laser radar system using resonance absorption for detection of air pollutants.